


0010010

x330 Series

Gigabit Layer 3 Access Switches

- x330-10GTX
- x330-20GTX
- x330-28GTX
- x330-52GTX

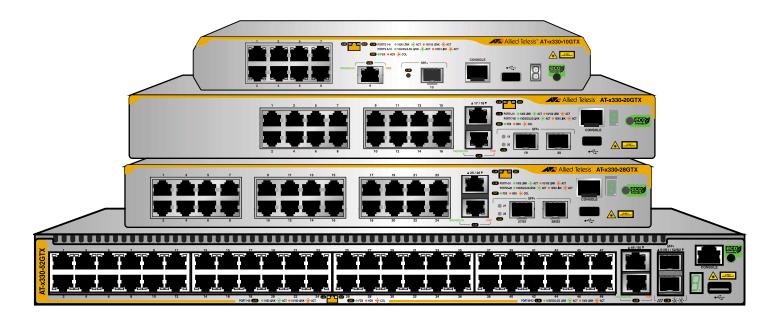

Installation Guide for Standalone Switches

Copyright © 2023 Allied Telesis, Inc.

All rights reserved. No part of this publication may be reproduced without prior written permission from Allied Telesis, Inc.

Allied Telesis, VCStack, and the Allied Telesis logo are trademarks of Allied Telesis, Incorporated. All other product names, company names, logos or other designations mentioned herein are trademarks or registered trademarks of their respective owners.

Allied Telesis, Inc. reserves the right to make changes in specifications and other information contained in this document without prior written notice. The information provided herein is subject to change without notice. In no event shall Allied Telesis, Inc. be liable for any incidental, special, indirect, or consequential damages whatsoever, including but not limited to lost profits, arising out of or related to this manual or the information contained herein, even if Allied Telesis, Inc. has been advised of, known, or should have known, the possibility of such damages.

This product meets the following standards.

U.S. Federal Communications Commission

Radiated Energy

Note: This equipment has been tested and found to comply with the limits for a Class A digital device pursuant to Part 15 of FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. This equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with this instruction manual, may cause harmful interference to radio communications. Operation of this equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference at his own expense.

Note: Modifications or changes not expressly approved of by the manufacturer or the FCC, can void your right to operate this equipment.

Industry Canada

This Class A digital apparatus complies with Canadian ICES-003.

Cet appareil numérique de la classe A est conforme à la norme NMB-003 du Canada.



Warning

In a domestic environment this product may cause radio interference in which case the user may be required to take adequate measures. & E84

Electrical Safety: EN 62368-1 (UL/EN/IEC)

	/	١	
,	ş	é	
/	17	5	Λ.

Laser Safety EN 60825-1

Table 1 lists the product certificates.

Table 1. Product Certifications

Additional Certificates	CISPR Class A (Comité International Spécial des Perturbations Radioélectriques) RoHS Compliant
Australia/New Zealand	RCM (Regulatory Compliance Mark)
Common Criteria	NIAP (National Information Assurance Partnership)

European Economic Area (EEA)	CE (Conformité Européenne) WEEE (Waste Electrical and Electronic Equipment) RoHS (EU 1025/863) (Restriction of Hazardous Substances)
European Standards (EN)	EMC (Immunity): EN 55024, EN 55035 Laser Safety: EN 60825-1 EN 55032 Class A, EN 61000-3-2, EN 61000-3-3
India	TEC (Telecommunications Engineering Center)
Japan	VCCI Class A (Voluntary Control Council for Interference)
Mexico	NOM (Normas Oficiales Mexicanas)
North America	FCC Class A Laser Safety: EN 60825-1 _C UL _{US} Energy Star
United Kingdom	UKCA (UK Conformity Assessment)

Table 1. Product Certifications (Continued)

Translated Safety Statements

Important: Safety statements with the *Arch* symbol are translated into multiple languages in **Translated Safety Statements** at **alliedtelesis.com/library/search**.

Übersetzte Sicherheitshinweise

Wichtig: Sicherheitshinweise mit dem & -Symbol werden in Translated Safety Statements bei alliedtelesis.com/library/search in mehrere Sprachen übersetzt.

Declaraciones de seguridad traducidas

Importante: Las declaraciones de seguridad con el símbolo *&* se traducen a varios idiomas en **Translated Safety Statements** en **alliedtelesis.com/library/search**.

Consignes de sécurité traduites

Important: Les déclarations de sécurité avec le symbole *ar* sont traduites en plusieurs langues en **Translated Safety Statements** sur **alliedtelesis.com/library/search**.

Dichiarazioni di sicurezza tradotte

Importante: Le dichiarazioni di sicurezza con il simbolo *&* sono tradotte in più lingue in **Translated Safety Statements** su **alliedtelesis.com/library/search**.

Översatta säkerhetsförklaringar

Viktig: Säkerhetsföreskrifter med & -symbolen översätts till flera språk på Translated Safety Statements vid alliedtelesis.com/library/search.

Contents

Preface	13
Document Conventions	14
Contacting Allied Telesis	15
Chapter 1: Overview	
Front and Back Panels	
Features	21
10/100/1000Mbps Copper Ports	21
1/2.5/5/10Gbps Multi-Gigabit Copper Ports	21
1/10Gbps SFP+ Ports	21
Port and System LEDs	
Installation Options	
MAC Address Table	
Management Software and Interfaces	23
Energy Savings	23
10/100/1000Mbps Copper Ports	24
1/2.5/5/10Gbps Multi-Gigabit Copper Ports	
SFP+ Ports	
Port LEDs	29
10/100/1000Mbps Copper Port LEDs	
1/2.5/5/10Gbps Multi-Gigabit Copper Port LEDs	
1/10Gbps SFP+ Port LEDs	
eco-friendly Button	34
Switch ID LED	
USB Port	
Console Port	
Power Supply and Power Savings Features	
Chapter 2: Beginning the Installation	
Reviewing Safety Precautions	42
Choosing a Site for the Switch	46
Site Requirements	
Enclosure Requirements	
Unpacking the Switch	
Installation Options	
x330-10GTX Switch	
x330-20GTX Switch	
x330-28GTX Switch	
x330-52GTX Switch	
Hardware Options	
RKMT-J05 Equipment Rack Brackets Kit	
BRKT-J23 Wall Brackets Kit	
RKMT-J13 Equipment Rack Brackets Kit	
BRKT-J24 Wall Brackets Kit	
Recording the Serial Number and MAC Address	
Installing the Switch on a Table	59
Chapter 3: Installing the x330-10GTX Switch in an Equipment Rack	
Introduction	
Installing the x330-10GTX Switch	66

Chapter 4: Installing the x330-20GTX Switch in an Equipment Rack	
Installing the x330-20GTX Switch	
Chapter 5: Installing the x330-28GTX Switch in an Equipment Rack	
Installing the x330-28GTX Switch	
Chapter 6: Installing the x330-52GTX Switch in an Equipment Rack	
Introduction	
Installing the x330-52GTX Switch	83
Chapter 7: Installing the x330-10GTX Switch on a Wall	
Introduction	
Installation Guidelines	
Installing the x330-10GTX Switch	89
Chapter 8: Installing x330-20GTX, x330-28GTX, and x330-52GTX Switches on a Wall	
Installation Guidelines	
Plywood Base for a Wall with Wooden Studs	
Installing the Switch	
Chapter 9: Verifying the Switch	
Powering On the Switch	
Starting a Management Session	
With a DHCP or DHCPv6 Server	
Without a DHCP or DHCPv6 Server	
Displaying the Hardware Status and Disabling VCStack	113
Chapter 10: Cabling Copper and SFP+ Ports	117
Cabling Copper Ports	
Guidelines to Handling SFP and SFP+ Transceivers	
Installing 1Gbps SFP and 10Gbps SFP+ Transceivers	
Installing AT-SP10TW Direct Connect Twinax Cables in SFP+ Ports	123
Chapter 11: Troubleshooting	125
Appendix A: Technical Specifications	
Physical Specifications	
Environmental Specifications	
Power Specifications	
RJ-45 Copper Port Pinouts	
RJ-45 Style Serial Console Port Pinouts	

Figures

	10
Figure 1: Front Panel of the x330-10GTX Switch Figure 2: Front Panel of the x330-20GTX Switch	
Figure 3: Front Panel of the x330-28GTX Switch	
Figure 4: Front Panel of the x330-52GTX Switch	
Figure 5: Back Panels	
Figure 6: Speed/Activity and Duplex Mode LEDs for the 10/100/1000Mbps Copper Ports	
Figure 7: Speed/Activity LEDs for the 1/2.5/5/10Gbps Multi-Gigabit Copper Ports	
Figure 8: Speed/Activity LEDs for the 1/10Gbps SFP+ Ports	
Figure 9: Switch ID LED	
Figure 10: Switch ID LED with eco-friendly Mode Off (Port LEDs On)	
Figure 11: Switch ID LED with eco-friendly Mode On (Port LEDs Off)	
Figure 12: Accessory Items Included with the x330-10GTX and x330-20GTX Switches	
Figure 13: Accessory Items Included with the x330-28GTX Switch	
Figure 14: Accessory Items Included with the x330-52GTX Switch	
Figure 15: Installation Options for the x330-10GTX Switch	
Figure 16: Installation Options for the x330-20GTX Switch	
Figure 17: Installation Options for the x330-28GTX Switch	
Figure 18: Installation Options for the x330-52GTX Switch	
Figure 19: RKMT-J05 Equipment Rack Brackets Kit for the x330-10GTX Switch	
Figure 20: BRKT-J23 Wall Brackets Kit for the x330-10GTX Switch	
Figure 21: RKMT-J13 Equipment Rack Brackets Kit for the x330-20GTX Switch	
Figure 22: BRKT-J24 Wall Brackets Kit for the x330-20GTX and x330-28GTX Switches	
Figure 23: Serial Number and MAC Address Labels	
Figure 24: x330 Switches Installation on a Table	
Figure 25: Unsupported Table Installations	
Figure 26: Attaching Bumper Feet on x330-10GTX, x330-20GTX, and x330-28GTX Switches	
Figure 27: Attaching Bumper Feet on the x330-52GTX Switch	
Figure 28: x330-10GTX Switch in an Equipment Rack with the RKMT-J05 Brackets Kit	
Figure 29: x330-10GTX Switch with RKMT-J05 Cable Trays	
Figure 30: Attaching the RKMT-J05 Handles to the Short Brackets	
Figure 31: Attaching the Short RKMT-J05 Brackets to the Long Brackets	
Figure 32: Attaching the RKMT-J05 Cord Trays to the Long Brackets	
Figure 33: Attaching the RKMT-J05 Brackets to the Switch	
Figure 34: Attaching the x330-10GTX Switch to the Equipment Rack	
Figure 35: x330-20GTX Switch with RKMT-J13 Equipment Rack Brackets Kit	
Figure 36: Attaching the Handles to the RKMT-J13 Brackets	
Figure 37: Attaching the Extenders to the RKMT-J13 Brackets	
Figure 38: Attaching the RKMT-J13 Brackets to the x330-20GTX Switch	74
Figure 39: Securing the x330-20GTX Switch in a Standard 19-inch Equipment Rack	75
Figure 40: x330-28GTX Switch in Standard 19-inch Equipment Racks	
Figure 41: Attaching the Equipment Rack Brackets to the x330-28GTX Switch	
Figure 42: Securing the x330-28GTX Switch in a Standard 19-inch Equipment Rack	
Figure 43: Bracket Screw Holes on the x330-52GTX Switch	
Figure 44: Equipment Rack Bracket Positions for the x330-52GTX Switch	
Figure 45: Attaching the Equipment Rack Brackets to the x330-52GTX Switch	
Figure 46: Securing the x330-52GTX Switch in a Standard 19-inch Equipment Rack	
Figure 47: x330-10GTX Switch with Two BRKT-J23 Wall Brackets	
Figure 48: x330-10GTX Switch with Four BRKT-J23 Wall Brackets	
Figure 49: Unsupported Wall Installation with Front Panel Facing Down	

Figures

Figure 50: Marking the Screw Holes for Two BRKT-J23 Brackets	90
Figure 51: Marking the Screw Holes for Four BRKT-J23 Brackets	91
Figure 52: Attaching the Bottom BRKT-J23 Brackets to the Wall	92
Figure 53: Sliding the Switch into the BRKT-J23 Brackets	93
Figure 54: Attaching the Top BRKT-J23 Brackets to the Wall	
Figure 55: x330-20GTX and x330-28GTX Switches on a Wall with the AT-BRKT-J24 Brackets Kit	96
Figure 56: x330-52GTX Switch on a Wall	96
Figure 57: Unsupported Wall Installation for the x330-20GTX, x330-28GTX, and x330-52GTX Switches	97
Figure 58: x330 Switch on a Wall with a Plywood Base	
Figure 59: Steps to Installing x330 Switches on a Plywood Base	100
Figure 60: Attaching the AT-BRKT-J24 Wall Brackets to x330-20GTX and x330-28GTX Switches	102
Figure 61: Attaching the Wall/Equipment Rack Brackets to the x330-52GTX Switch	102
Figure 62: Attaching the Wall/Equipment Rack Brackets to the x330-52GTX Switch (continued)	103
Figure 63: Marking the Locations of the Bracket Holes	104
Figure 64: Installing the Power Cord Retaining Clip	106
Figure 65: Connecting the AC Power Cord	106
Figure 66: Lowering the Power Cord Retaining Clip	107
Figure 67: Connecting the Power Cord to an AC Power Source	107
Figure 68: Management Cable Included with Switch	
Figure 69: VT-Kit3 Management Cable	108
Figure 70: Local Management with the VT-Kit3 Management Cable	109
Figure 71: Moving to the Global Configuration Mode	113
Figure 72: Confirmation Prompt for the NO STACK ENABLE Command	114
Figure 73: Returning to the Privileged Exec Mode	114
Figure 74: Saving the Changes with the WRITE Command	114
Figure 75: Installing an SFP+ Transceiver	
Figure 76: Removing the Dust Cover from an SFP+ Transceiver	
Figure 77: Positioning the SFP+ Handle in the Upright Position	
Figure 78: Connecting a Fiber Optic Cable to an SFP or SFP+ Transceiver	
Figure 79: Installing an AT-SP10TW Cable	
Figure 80: Dimensions of the x330-10GTX Switch	
Figure 81: Dimensions of x330-20GTX and x330-28GTX Switches	131
Figure 82: Dimensions of the x330-52GTX Switch	
Figure 83: Bracket Screw Holes on the x330-20GTX and x330-28GTX Switches	
Figure 84: Bracket Screw Holes on the x330-52GTX Switch	
Figure 85: Pin Layout for the RJ-45 Copper Ports (Front View)	139

Tables

Table 1: Product Certifications	3
Table 2: Specifications of the 10/100/1000Mbps Copper Ports	24
Table 3: Specifications of the 1/2.5/5/10Gbps Multi-Gigabit Copper Ports	26
Table 4: Speed/Activity LEDs for the 10/100/1000Mbps Copper Ports	
Table 5: Duplex Mode LEDs for the 10/100/1000Mbps Copper Ports	
Table 6: Speed/Activity LEDs for the 1/2.5/5/10Gbps Multi-Gigabit Copper Ports	31
Table 7: Speed/Activity LEDs for the 1/10Gbps SFP+ Ports	33
Table 8: Product Dimensions (H x W x D)	
Table 9: Switch Weights	
Table 10: Ventilation Requirements	
Table 11: Environmental Specifications	
Table 12: Maximum Power Consumption	
Table 13: Input Voltages	
Table 14: Heat Dissipation	
Table 15: Product Certifications	
Table 16: Pin Signals for Copper Ports	
Table 17: RJ-45 Style Serial Console Port Pin Signals	

Tables

Preface

This guide contains the hardware installation instructions for the x330 Series of Gigabit Layer 3 access switches as standalone units. The preface contains the following sections:

- □ "Document Conventions" on page 14
- Contacting Allied Telesis" on page 15

The x330 Switches also support Virtual Chassis Stacking (VCStackTM). The feature allows you to manage multiple switches as a single unit and add redundancy to your network topology by distributing functions across multiple devices. For installation instructions, refer to the x330 Series Installation Guide for Virtual Chassis Stacking.

Document Conventions

This document uses the following conventions:

Note

Notes provide additional information.



Caution

Cautions inform you that performing or omitting a specific action may result in equipment damage or loss of data.



Warning

Warnings inform you that performing or omitting a specific action may result in bodily injury.

Contacting Allied Telesis

For assistance with this product, you may contact Allied Telesis technical support on the Services & Support section of the Allied Telesis web site at **www.alliedtelesis.com/us/en/services-support**. The page has links to the following services:

- Helpdesk (Support Portal) Log onto Allied Telesis interactive support center to search for answers to your questions in our knowledge database, check support tickets, learn about Return Merchandise Authorizations (RMAs), and contact Allied Telesis technical experts.
- Software Downloads Download the latest software releases for your product.
- Licensing Register and obtain your License key to activate your product.
- Product Documents View the most recent installation guides, user guides, software release notes, white papers and data sheets for your product.
- Warranty View a list of products to see if Allied Telesis warranty applies to the product you purchased and register your warranty.
- □ Allied Telesis Helpdesk Contact a support representative.

Preface

Chapter 1 Overview

This chapter contains the following sections:

- □ "Front and Back Panels" on page 18
- □ "Features" on page 21
- □ "10/100/1000Mbps Copper Ports" on page 24
- □ "1/2.5/5/10Gbps Multi-Gigabit Copper Ports" on page 26
- □ "SFP+ Ports" on page 28
- □ "Port LEDs" on page 29
- "eco-friendly Button" on page 34
- □ "Switch ID LED" on page 35
- □ "USB Port" on page 37
- □ "Console Port" on page 38
- □ "Power Supply and Power Savings Features" on page 39

Front and Back Panels

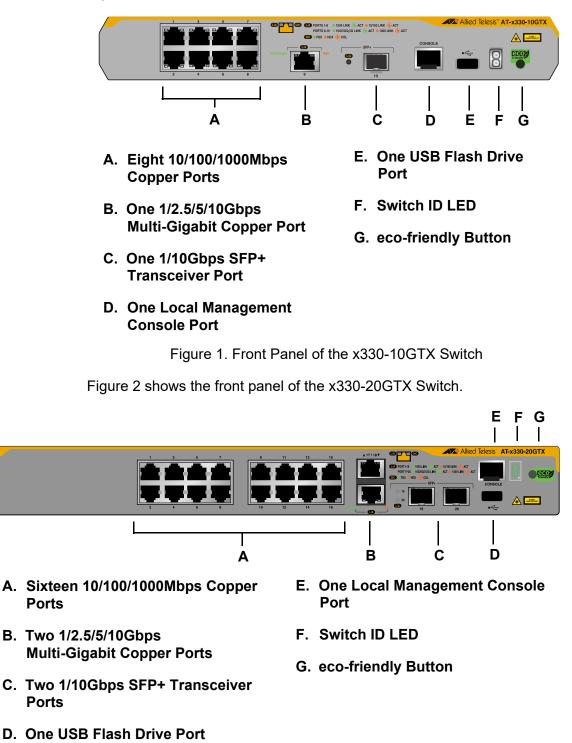


Figure 1 shows the front panel of the x330-10GTX Switch.

Figure 2. Front Panel of the x330-20GTX Switch

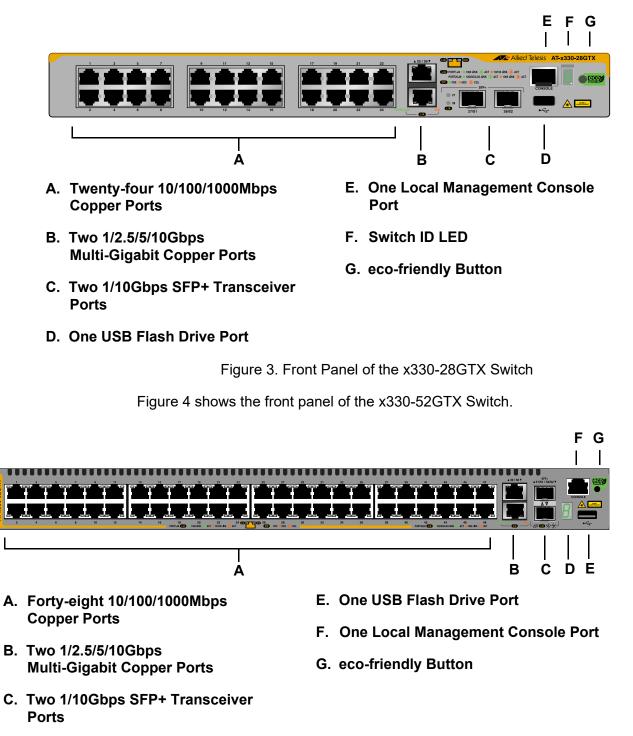


Figure 3 shows the front panel of the x330-28GTX Switch.

D. Switch ID LED

Figure 4. Front Panel of the x330-52GTX Switch

Figure 5 illustrates the back panels.

x330-10GTX Switch



x330-20GTX and x330-28GTX Switches



x330-52GTX Switch





Figure 5. Back Panels

Note

The x330-10GTX, x330-20GTX, and x330-28GTX Switches are fanless. The x330-52GTX Switch has a single fan inside the back panel. Its ventilation direction is from front to back. The fan draws air out of the device.

Features

10/100/1000Mbps	The ba	asic features of the 10/100/1000Mbps copper ports are listed here:
Copper Ports		10Base-T, 100Base-TX, and 1000Base-T compliant
		IEEE 802.3u Auto-Negotiation compliant
		Auto-MDI/MDIX
		100 meters (328 feet) maximum operating distance
		IEEE 802.3x flow control in 10/100Base-TX full-duplex mode
		IEEE 802.3x backpressure in 10/100Base-TX half-duplex mode
		Speed/activity LEDs
		Jumbo frames up to 12288 bytes
		RJ-45 connectors
1/2.5/5/10Gbps Multi-Gigabit	The ba listed l	asic features of the 1/2.5/5/10Gbps Multi-Gigabit copper ports are nere:
Copper Ports		1000Base-T, 2.5GBase-T, 5GBase-T, and 10GBase-T compliant
		IEEE 802.3bz for 2.5GBase-T and 5GBase-T
		Auto-Negotiation for speed
		100 meters (328 feet) maximum operating distance per port
		Full-duplex mode only
		Speed/activity LEDs
		RJ-45 connectors
1/10Gbps SFP+ Ports		FP+ ports support the following types of 1Gbps SFP and 10Gbps transceivers:
		1Gbps SFP 1000Base-SX/LX transceivers
		1Gbps SFP 1000Base-LX single-port BiDi transceivers
		1Gbps SFP 1000Base-ZX transceivers
		10Gbps SFP+ 10GBase-SR/LR fiber optic transceivers
		10Gbps SFP+ 1-meter AT-SP10TW1 and 3-meter AT-SP10TW3 direct connect twinax cables with SFP+ transceiver-style connectors
		10Gbps SFP+ single-port BiDi transceivers
		AT-SP10TM 1/2.5/5/10Gbps copper transceiver

Note

The SFP+ ports do not support 100Mbps 100Base-FX transceivers.

Note

The ports support full-duplex mode only.

Note

SFP and SFP+ transceivers are sold separately. Refer to the product's data sheet on the Allied Telesis website for a list of supported transceivers.

Note

The switches do not support the 7-meter AT-SP10TW7 direct connect twinax cable.

Port and System

Here are the port and system LEDs:

LEDs

- Speed/activity and duplex mode LEDs for the 10/100/1000Mbps copper ports
- □ Speed/activity LEDs for the 1/2.5/5/10Gbps Multi-Gigabit copper ports
- Speed/activity LEDs for the SFP+ ports
- Switch ID number LED

Note

Refer to "Port LEDs" on page 29.

Installation Here are the installation options for the switches:

	Desk	or	tab	letop
--	------	----	-----	-------

- Standard 19-inch equipment rack
- Wood or concrete wall

MAC Address Here are the basic features of the MAC address tables in the switches:

Table

Options

□ Storage capacity of 16,384 dynamic entries

- Storage capacity of 256 static entries
- Automatic learning and aging

Management	Here are the management software and interfaces:		
Software and		AlliedWare Plus Management Software	
Interfaces		Local management through the Console port	
		Remote Telnet and Secure Shell management	
		Remote HTTP and HTTPS web browser management	
		Command line interface	
		Autonomous Management Framework	
		Vista Manager EX	
		AMF-Security	
		SNMPv1, v2c, and v3	
Energy Savings	Here a	are energy saving features:	
		eco-friendly button for turning on and off the port LEDs	

□ IEEE 802.3az Energy-Efficient Ethernet (EEE)

10/100/1000Mbps Copper Ports

Table 1 lists the specifications of the 10/100/1000Mbps copper ports.

Feature	Description
Speeds	Port speeds are listed here: - 10Mbps (IEEE802.3 10Base-T) - 100Mbps (IEEE802.3u 100Base-TX) - 1Gbps (IEEE802.3ab 1000Base-T) Speeds are set manually or with IEEE 802.3u Auto-Negotiation.
Duplex modes	 Duplex modes are listed here: Half- or full-duplex mode at 10/100Mbps Full-duplex mode only at 1000Mbps Duplex modes are set manually or with IEEE 802.3u Auto-Negotiation. Speed and duplex mode settings of copper ports can be set independently of each other. For instance, ports can be configured such that their speeds are set manually while their duplex modes are set through Auto-Negotiation.
Wiring	Auto-MDI/MDIX at 10/100/1000Mbps (IEEE 802.3ab-compliant)
Maximum Distance	100 meters (328 feet)
Cable	 Cable requirements are listed here: 10/100Mbps - Standard TIA/EIA 568-B- compliant Category 3 unshielded cable or better. 1Gbps - Standard TIA/EIA 568-B-compliant Category 5 or Category 5e unshielded cable or better.

Table 1. Specifications of the 10/100/1000Mbps Copper Ports

Feature	Description
Additional Features	Additional features are listed here:
	- 8-pin RJ-45 connectors
	 Backpressure flow control supported at half- duplex mode
	 Non-blocking, wire speed supported at all speeds.
	- Jumbo frames up to 12288 bytes
	- 2MB packet buffer

Table 1. Specifications of the 10/100/1000Mbps Copper Ports (Continued)

For port pinouts, refer to "RJ-45 Copper Port Pinouts" on page 139.

Note

Copper ports must be set to Auto-Negotiation, the default, to function at 1000Mbps. The network devices must be IEEE 802.3u compliant.

Note

Copper ports that are connected to devices that do not support Auto-Negotiation should not use Auto-Negotiation to set speed and duplex mode. Otherwise, a speed or duplex mode mismatch might occur between the devices, resulting in reduced performance. You should set speed and duplex mode manually on copper ports that are connected to devices that do not support Auto-Negotiation.

1/2.5/5/10Gbps Multi-Gigabit Copper Ports

The x330-10GTX Switch has one Multi-Gigabit copper port. The x330-20GTX, x330-28GTX, and x330-52GTX Switches have two Multi-Gigabit copper ports. Table 2 lists the port specifications.

Specification	Description
Port Speed	Here are the supported speeds:
	- 1Gbps (IEEE802.3ab)
	- 2.5Gbps (IEEE 802.3bz)
	- 5Gbps (IEEE 802.3bz)
	- 10Gbps (IEEE 802.3an)
	You can set port speed with Auto- Negotiation or manually. Guidelines are given here:
	 1Gbps and 10Gbps can be set either manually or with Auto-Negotiation.
	 2.5Gbps and 5Gbps must be set with Auto-Negotiation.
	- The default setting is Auto-Negotiation.
Duplex Mode	Full-duplex only
Maximum Distance	100 meters (328 feet)
Connector	8-pin RJ-45
Cable Requirements	 1/2.5/5Gbps - Standard TIA/EIA 568-A- compliant Category 5 or TIA/EIA 568-B- compliant Enhanced Category 5 (Cat 5e) unshielded cabling.
	 10Gbps -Standard TIA/EIA 568-C- compliant Category 6a unshielded cabling.

Specification	Description
Additional Features	Additional features are listed here:
	- 8-pin RJ-45 connectors
	 Non-blocking, wire speed supported at all speeds
	 Supports up to 12KB jumbo frames at 1/ 5/10Gbps
	 Supports up to 10KB jumbo frames at 2.5Gbps
	- 2MB packet buffer

Table 2. Specifications of the 1/2.5/5/10Gbps Multi-Gigabit Copper Ports

Note

Network devices connected to the Multi-Gigabit ports must be IEEE 802.3u compliant.

SFP+ Ports

The x330-10GTX Switch has one SFP+ port. The x330-20GTX, x330-28GTX, and x330-52GTX Switches have two SFP+ ports. The ports support the following types of 1Gbps SFP and 10Gbps SFP+ transceivers:

- IGbps SFP 1000Base-SX/LX transceivers
- IGbps SFP 1000Base-LX single-port BiDi transceivers
- IGbps SFP 1000Base-ZX transceivers
- 10Gbps SFP+ 10GBase-SR/LR fiber optic transceivers
- 10Gbps SFP+ 1-meter AT-SP10TW1 and 3-meter AT-SP10TW3 direct connect twinax cables with SFP+ transceiver-style connectors
- 10Gbps SFP+ single-port BiDi transceivers
- AT-SP10TM 1/2.5/5/10Gbps copper port transceiver

You can use the ports to connect switches to other network devices over large distances, build a high-speed backbone network between network devices, or connect high-speed devices, such as servers, to your network.

Note

The SFP+ ports do not support 100Mbps 100Base-FX transceivers.

Note

The ports support full-duplex mode only.

Note

SFP and SFP+ transceivers are sold separately. Refer to the product's data sheet for a list of supported transceivers.

Note

The switches do not support the 7-meter SFP+ AT-SP10TW7 direct connect twinax cable.

Port LEDs

This section describes the copper, Multi-Gigabit, and SFP+ port LEDs.

10/100/1000Mbps Copper Port LEDs

The 10/100/1000Mbps copper ports have two LEDs that display the following information:

- Speed/activity
 - □ Duplex mode

The LEDs are identified in Figure 6.

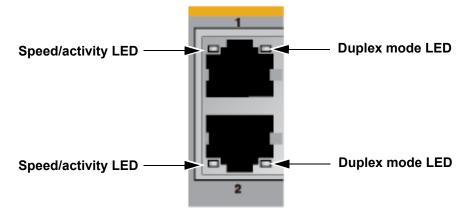


Figure 6. Speed/Activity and Duplex Mode LEDs for the 10/100/1000Mbps Copper Ports

Table 3 and Table 4 on page 30 define the LEDs.

Table 3. Speed/Activity LEDs for the 10/100/1000Mbps Copper Ports

State	Description
Solid Green	The port has established a 1Gbps link to a network device.
Flashing Green	The port is transmitting or receiving network packets at 1Gbps.
Solid Amber	The port has established a 10 or 100Mbps link to a network device.
Flashing Amber	The port is transmitting or receiving network packets at 10 or 100Mbps.

State	Description
Off	Possible causes of this state are listed here:
	 The port has not established a link with another network device.
	- The LEDs are turned off. To turn on the LEDs, use the eco-friendly button.

Table 4 describes the duplex mode LEDs for the 10/100/1000Mbps copper ports.

Table 4. Duplex Mode LEDs for the 10/100/1000Mbps Copper Ports

State	Description
Solid Green	The port is operating in full duplex mode.
Solid Amber	The port is operating in half duplex mode.
Flashing Amber	The port is operating in half duplex mode, with collisions.
Off	Possible causes of this state are listed here:
	 The port has not established a link with another network device.
	- The LEDs are turned off. To turn on the LEDs, use the eco-friendly button.


 1/2.5/5/10Gbps
 The 1/2.5/5/10Gbps Multi-Gigabit copper ports have two LEDs that display speed/activity information. Refer to Figure 7.

 LEDs
 2.5/5/10Gbps

 LED
 1Gbps

 LED
 1Gbps



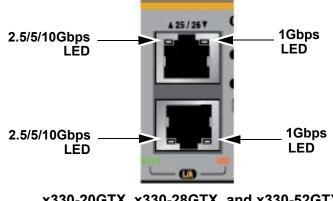

x330-20GTX, x330-28GTX, and x330-52GTX Switches

Figure 7. Speed/Activity LEDs for the 1/2.5/5/10Gbps Multi-Gigabit Copper Ports

Table 5 describes the LEDs.

Table 5. Speed/Activity LEDs for the 1/2.5/5/10Gbps Multi-Gigabit Copper Ports

State	Description
Solid Green (left LED)	The port has established a 2.5Gbps, 5Gbps, or 10Gbps link to a network device.
Flashing Green (left LED)	The port is transmitting or receiving data at 2.5Gbps, 5Gbps, or 10Gbps.
Solid Amber (right LED)	The port has established a 1Gbps link to a network device.
Flashing Amber (right LED)	The port is transmitting or receiving data at 1Gbps.

State	Description
Off	Possible causes of this state are listed here:
	 The port has not established a link with another network device.
	 The LEDs are turned off. To turn on the LEDs, use the eco-friendly button.

Table 5. Speed/Activity LEDs for the 1/2.5/5/10Gbps Multi-Gigabit Copper Ports (Continued)

1/10Gbps SFP+
Port LEDsThe 1/10Gbps SFP+ ports have one LED that displays speed/activity
information. Refer to Figure 8.



x330-10GTX Switch



x330-20GTX and x330-28GTX Switches



x330-52GTX Switch

Figure 8. Speed/Activity LEDs for the 1/10Gbps SFP+ Ports

Table 6 describes the LED.

Table 6. Speed/Activity LEDs for the 1/10Gbps SFP+ Ports

State	Description
Solid Amber	The port has established a 1Gbps link to a network device.
Flashing Amber	The port is transmitting or receiving data at 1Gbps.
Solid Green	The port has established a 10Gbps link to a network device.
Flashing Green	The port is transmitting or receiving data at 10Gbps.
Off	Possible causes of this state are listed here:
	 The port has not established a link with another network device.
	- The LEDs are turned off. To turn on the LEDs, use the eco-friendly button.

eco-friendly Button

You use the eco-friendly button on the front panel of the switch to toggle the port LEDs on and off. You can conserve electricity by turning off the LEDs when you are not monitoring the device. When the LEDs are turned off, the switch is operating in the low power eco-friendly mode. Turning off the port LEDs does not interfere with the network operations of the switch. When the switches are operating in a stack, pressing the eco-friendly button toggles the eco-friendly mode on all the stack switches.

You can also toggle the port LEDs on and off with the ECOFRIENDLY LED and NO ECOFRIENDLY LED commands in the Global Configuration mode in the command line interface of the AlliedWare Plus management software, as follows:

- □ ECOFRIENDLY LED command Turns off the LEDs.
- □ NO ECOFRIENDLY LED command Turns on the LEDs.

The AlliedWare Plus management software has a command that blinks all the port LEDs so that you can quickly identify a specific unit among the devices in an equipment rack. It is the FINDME command. The command works even if the port LEDs are turned off.

The Switch ID LED is always on. It displays different information depending on whether the port LEDs are on or off. When the port LEDs are on, the Switch ID LED displays the ID number of the switch in a VCStack. When the switch is operating in the low power mode with the port LEDs off, the Switch ID LED indicates whether the switch is the master or member switch of a VCStack. Refer to "Switch ID LED" on page 35.

Note

Before checking or troubleshooting network connections to the ports on the switch, you should verify that the LEDs are on by pressing the eco-friendly button or issuing the NO ECOFRIENDLY LED command in the Global Configuration mode of the command line interface.

Switch ID LED

The Switch ID LED, shown in Figure 9, is for the VCStack feature for the x330-20GTX, x330-28GTX, and x330-52GTX Switches. With VCStack, you can manage up to six switches as a single unit. This simplifies network management and allows you to add redundancy to your network topology by distributing functions across multiple switches.



Figure 9. Switch ID LED

The LED displays different information depending on whether the low power eco-friendly mode is on or off. Refer to "eco-friendly Button" on page 34. Figure 10 lists the states of the LED when the eco-friendly mode is off and the port LEDs are on.



The switch is booting up.



The switch has detected a fault condition, such as overheating.



VCStack is disabled. The switch is a standalone unit.



VCStack is enabled. The switch has an ID number in the range of 1 to 6.



Flashing dot in the lower right corner indicates the switch is accessing a USB flash drive.

Figure 10. Switch ID LED with eco-friendly Mode Off (Port LEDs On)

Note

The x330-10GTX Switch does not support the VCStack feature. It operates as a standalone device and displays "0" on the Switch ID LED when the eco-friendly mode is off.

Note

If the Switch ID LED displays "F" for a fault condition, use the SHOW SYSTEM ENVIRONMENT command in the command line interface of the AlliedWare Plus management software to identify the source of the problem.

Figure 11 illustrates the states of the LED when the eco-friendly mode is on and the port LEDs are off.



The switch is the master switch of a VCStack.



The switch is a standalone unit.



The switch is a member switch of a VCStack.

Figure 11. Switch ID LED with eco-friendly Mode On (Port LEDs Off)

You use the USB port to store configuration files on flash drives to maintain a history of the switch's configurations, or to restore configuration files to the switch. You can also use the port and flash drives to quickly configure replacement units and update the AlliedWare Plus management software.

The port is USB 2.0 compatible.

Console Port

You use the Console port to configure the features and parameter settings of the switch with the command line interface in the AlliedWare Plus management software. This management is called local management because it is not conducted over your network. You have to be at the physical location of the switch. The Console port has these settings:

- Default baud rate: 9600 bps (Range is 9600 to 115200 bps)
- Data bits: 8
- Parity: None
- □ Stop bits: 1
- □ Flow control: None

Note

These settings are for a DEC VT100 or ANSI terminal, or an equivalent terminal emulation program.

Local management sessions require a management cable for connecting your computer or terminal to the Console port. Here are the cable guidelines:

- If your computer has an RS-232 port, you may use the management cable supplied with the switch. Refer to Figure 12 on page 48. The cable has RJ-45 and DB-9 connectors.
- If your computer has a USB port, you may need to purchase a USB-to-Serial converter that is compatible with its operating system. An example is the VT-Kit3 from Allied Telesis.

The Console port pinouts are provided in "RJ-45 Style Serial Console Port Pinouts" on page 140. For further information, refer to "Starting a Management Session" on page 108.

Power Supply and Power Savings Features

The x330 Switches have one internal power supply. The power supply is not field-replaceable. Refer to "Power Specifications" on page 135 for the input voltage ranges.



Warning

Power cord is used as a disconnection device. To de-energize equipment, disconnect the power cord. Ger E3

The switches support the following power savings features:

- The switch supports IEEE 802.3az Energy-Efficient Ethernet (EEE). EEE is an energy saving feature that reduces power consumption during periods of no data activity. The switch saves electricity by placing the Ethernet circuitry in a special sleep mode when all the ports are inactive. When data activity resumes, the circuitry automatically resumes normal operations.
- □ The switches include the eco-friendly mode for turning off port LEDs to save power. Refer to "eco-friendly Button" on page 34.

Chapter 1: Overview

Chapter 2 Beginning the Installation

The chapter contains the following sections:

- □ "Reviewing Safety Precautions" on page 42
- □ "Choosing a Site for the Switch" on page 46
- □ "Unpacking the Switch" on page 48
- □ "Installation Options" on page 51
- □ "Hardware Options" on page 55
- □ "Recording the Serial Number and MAC Address" on page 58
- □ "Installing the Switch on a Table" on page 59

Reviewing Safety Precautions

Review the following safety precautions before beginning the installation procedure.

Note

Safety statements that have the *correct symbol* are translated into multiple languages in the *Translated Safety Statements* document at **www.alliedtelesis.com/en/documents/translated-safety-statements**.

Note

Les consignes de sécurité portant le symbole & sont traduites dans plusieurs langues dans le document *Translated Safety Statements,* disponible à l'adresse **www.alliedtelesis.com/en/ documents/translated-safety-statements**.



Warning

Class 1 Laser product. & L1



Warning

Do not stare into the laser beam. & L2



Warning

Do not look directly at the fiber optic cable ends or inspect the cable ends with an optical lens. & L6



Warning

To prevent electric shock, do not remove the cover. No userserviceable parts inside. This unit contains hazardous voltages and should only be opened by a trained and qualified technician. To avoid the possibility of electric shock, disconnect electric power to the product before connecting or disconnecting the LAN cables. α E1



Warning

Do not work on equipment or cables during periods of lightning activity. $\alpha \sim E2$



Warning

Power cord is used as a disconnection device. To de-energize equipment, disconnect the power cord. \nleftrightarrow E3



Warning

Class I Equipment. This equipment must be earthed. The power plug must be connected to a properly wired earth ground socket outlet. An improperly wired socket outlet could place hazardous voltages on accessible metal parts. & E4

Note

Pluggable Equipment. The socket outlet shall be installed near the equipment and shall be easily accessible. & E5



Caution

Air vents must not be blocked and must have free access to the room ambient air for cooling. & E6



Warning

Operating Temperatures. This product is designed for a maximum ambient temperature of 45 degrees C. & E57

Note

All Countries: Install product in accordance with local and National Electrical Codes. & E8



Warning

Only trained and qualified personnel are allowed to install or replace this equipment. ω E14



Caution

Circuit Overloading: Consideration should be given to the connection of the equipment to the supply circuit and the effect that overloading of circuits might have on overcurrent protection and supply wiring. Appropriate consideration of equipment nameplate ratings should be used when addressing this concern. α E21



Caution

Risk of explosion if battery is replaced by an incorrect type. Replace only with the same or equivalent type recommended by the manufacturer. Dispose of used batteries according to the manufacturer's instructions. $\alpha \sim E22$



Warning

Mounting of the equipment in the rack should be such that a hazardous condition is not created due to uneven mechanical loading. & E25

Note

Use dedicated power circuits or power conditioners to supply reliable electrical power to the device. & E27



Caution

The chassis may be heavy and awkward to lift. Allied Telesis recommends that you get assistance when mounting the chassis in an equipment rack. & E28

Note

If installed in a closed or multi-unit rack assembly, the operating ambient temperature of the rack environment may be greater than the room ambient temperature. Therefore, consideration should be given to installing the equipment in an environment compatible with the manufacturer's maximum rated ambient temperature (Tmra). \approx E35



Caution

Installation of the equipment in a rack should be such that the amount of air flow required for safe operation of the equipment is not compromised. & E36



Warning

Reliable earthing of rack-mounted equipment should be maintained. Particular attention should be given to supply connections other than direct connections to the branch circuits (e.g., use of power strips). $\approx E37$



Caution

The unit does not contain serviceable components. Please return damaged units for servicing. & E42



Warning

The temperature of an active SFP transceiver may exceed 40° C (158° F). Exercise caution when handling with unprotected hands. α E43



Caution

You have to reset the switch to disable the VCStack feature. Some network traffic may be lost if the device is already connected to a live network. ω E75



Warning

Switches should not be stacked on top of one another on a table or desktop because that could present a personal safety hazard if you need to move or replace switches. \swarrow E76



Warning

A transceiver can be damaged by static electricity. Be sure to observe all standard electrostatic discharge (ESD) precautions, such as wearing an anti-static wrist strap, to avoid damaging the device. \swarrow E77

Choosing a Site for the Switch

Site and enclosure requirements are described in the following sections:

- □ "Site Requirements," next
- "Enclosure Requirements" on page 47
- **Site** Observe these site requirements when planning the installation.

Requirements

- □ The x330-10GTX, x330-20GTX, and x330-28GTX Switches are fanless.
- The x330-52GTX Switch has a single internal fan on the rear panel. Its airflow direction is from front to back, with the fan pulling air out of the chassis.
- You should verify that the temperature range and ventilation at the installation site are suitable for the devices, and that there is adequate air flow around the units for cooling. The operating temperature range of the switches is provided in "Environmental Specifications" on page 134.
- If you plan to install the switch in an equipment rack, verify that the rack is safely secured so that it will not tip over. Devices in a rack should be installed starting at the bottom, with the heavier devices near the bottom of the rack.
- If you plan to install the switch on a table, verify that the table is level and stable.
- □ The power outlet should be located near the switch and be easily accessible.
- The site should allow for easy access to the ports on the front of the switch, so that you can easily connect and disconnect cables, and view the port LEDs.
- Do not install the switch in a wiring or utility box without adequate airflow. The switch might overheat and fail. Refer to "Enclosure Requirements" on page 47.
- **The site should not expose the switch to moisture or water.**
- □ The site should be a dust-free environment.
- The site should include dedicated power circuits or power conditioners to supply reliable electrical power to the network devices.
- The site should not expose the copper cabling to sources of electrical noise, such as radio transmitters, broadband amplifiers, power lines, electric motors, and fluorescent fixtures.
- Switch ports are suitable for intra-building connections, or where non-exposed cabling is required.

Do not place objects on top of the switch.



Warning

Switches should not be stacked on top of one another on a table or desktop because that could present a personal safety hazard if you need to move or replace switches. α E76

Observe these guidelines when installing the switch in an enclosure:

Requirements

Enclosure

- Verify that the enclosure has adequate airflow so that unit does not overheat.
- □ Select an enclosure that is large enough for the switch and all other included equipment.
- □ The enclosure size must be determined by considering multiple factors, including the outside ambient temperature, total heat generated by the installed equipment, sealed or unsealed enclosure type, enclosure material, paint color, mounting method (wall, pole, ground, etc.), and sun exposure. The smaller enclosure size you choose, the higher the risk of overheating the product faces.

Note

If the product overheats in an enclosure that was selected without taking into account these factors, the warranty of the product might be voided. Consult Allied Telesis when assistance is needed.

- The enclosure's BTU/hour rating must be higher than the total BTU/hour values of installed equipment, over the expected operating temperature range. For the operating temperature ratings, refer to Table 10, "Environmental Specifications" on page 134.
- Be sure to review the enclosure's installation guide for rules and restrictions on site requirements, and to follow all guidelines and safety warnings.

Unpacking the Switch

The x330-10GTX and x330-20GTX Switches come with the accessory items in Figure 12.

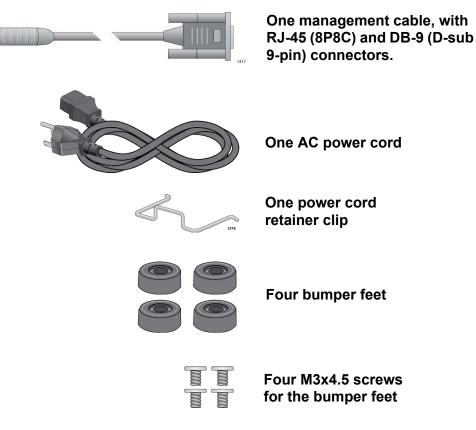


Figure 12. Accessory Items Included with the x330-10GTX and x330-20GTX Switches

Note

Please retain the original packaging material in the event you need to return the unit to Allied Telesis.

The x330-28GTX Switch comes with the accessory items in Figure 13.


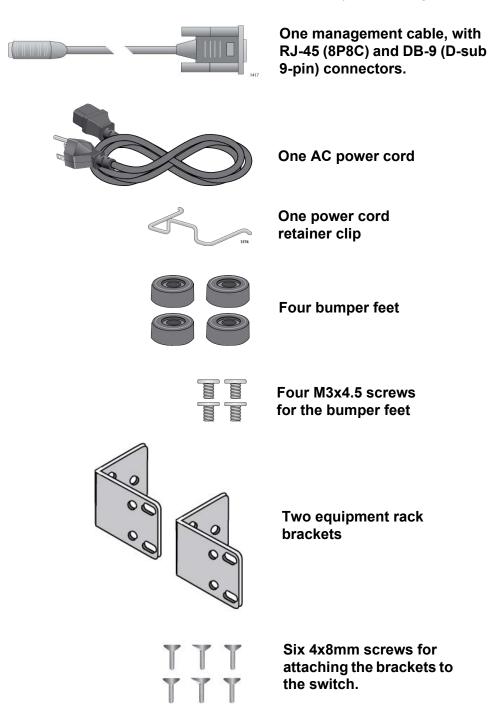


Figure 13. Accessory Items Included with the x330-28GTX Switch

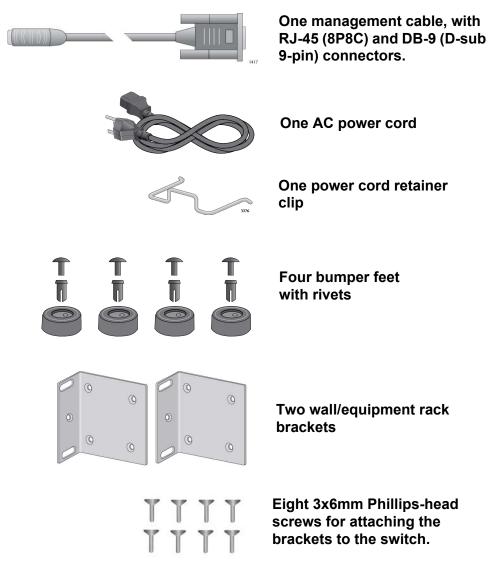

The x330-52GTX Switch comes with the accessory items Figure 14.

Figure 14. Accessory Items Included with the x330-52GTX Switch


Installation Options

The following sections illustrate the installation options for the switches.

x330-10GTX Figure 15 illustrates the installation options for the x330-10GTX Switch. Switch




Table or desktop with the bumper feet included with switch.

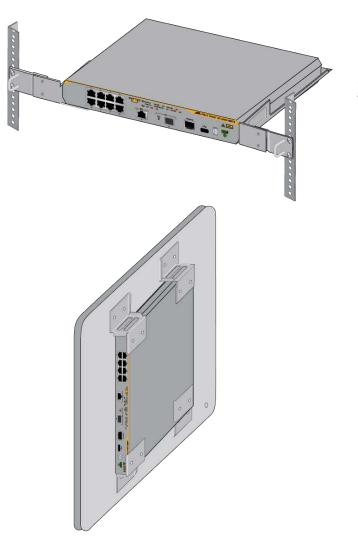

Standard 19-inch equipment rack with the RKMT-J05 equipment rack brackets kit. Kit sold separately.


Wall installation with the BRKT-J23 wall brackets kit. Kit sold separately.


Figure 15. Installation Options for the x330-10GTX Switch

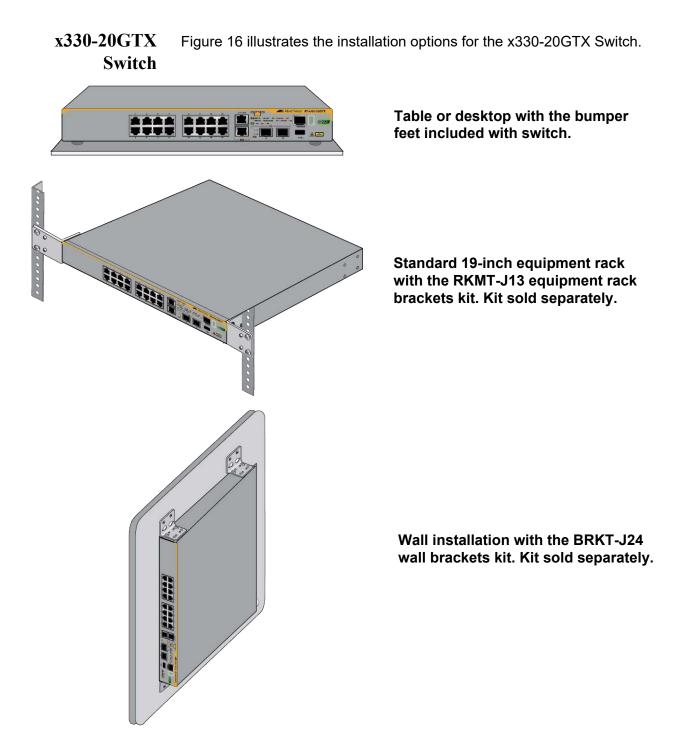



x330-28GTX Figure 17 illustrates the installation options for the x330-28GTX Switch. Switch

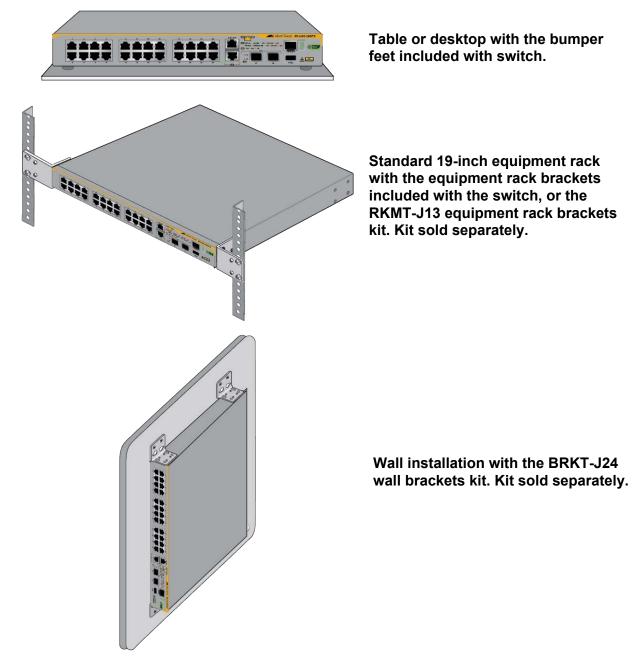



x330-52GTX Figure 18 illustrates the installation options for the x330-52GTX Switch. Switch

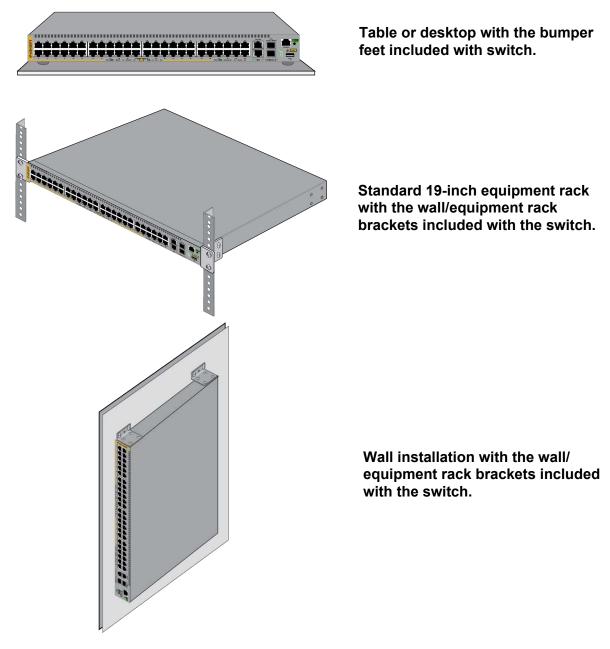


Figure 18. Installation Options for the x330-52GTX Switch

Hardware Options

The following hardware options are sold separately.

Note The x330-52GTX Switch does not require the hardware options.

RKMT-J05 Equipment Rack Brackets Kit

Installing the x330-10GTX Switch in a standard 19-inch equipment rack requires the RKMT-J05 brackets kit. Refer to Figure 19. For instructions, refer to Chapter 3, "Installing the x330-10GTX Switch in an Equipment Rack" on page 63.

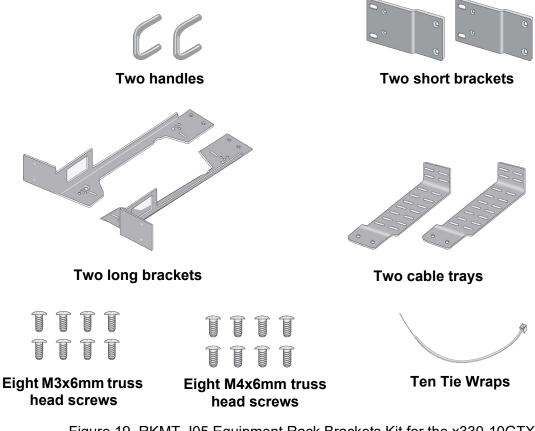


Figure 19. RKMT-J05 Equipment Rack Brackets Kit for the x330-10GTX Switch

BRKT-J23 Wall Brackets Kit

The x330-10GTX Switch is installed on a wall with the BRKT-J23 wall brackets kit. Refer to Figure 20. For instructions, refer to Chapter 7, "Installing the x330-10GTX Switch on a Wall" on page 85.




Figure 20. BRKT-J23 Wall Brackets Kit for the x330-10GTX Switch

RKMT-J13 Equipment Rack Brackets Kit

Installing the x330-20GTX Switch in a standard 19-inch equipment rack requires the RKMT-J13 brackets kit, shown in Figure 21. You can install the switch with the front panel flush with or recessed 50mm (2 in.) behind the front of the equipment rack. For instructions, refer to Chapter 4, "Installing the x330-20GTX Switch in an Equipment Rack" on page 71.

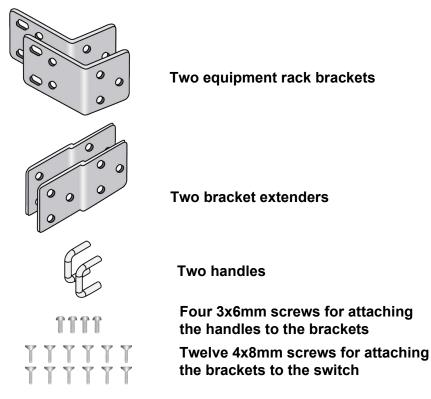


Figure 21. RKMT-J13 Equipment Rack Brackets Kit for the x330-20GTX Switch

Note

The x330-28GTX and x330-52GTX Switches come with brackets for equipment rack installations.

BRKT-J24 Wall Brackets Kit

Installing x330-20GTX and x330-28GTX Switches on a wall requires the BRKT-J24 wall brackets kit. Refer to Figure 22. For instructions, refer to Chapter 8, "Installing x330-20GTX, x330-28GTX, and x330-52GTX Switches on a Wall" on page 95.

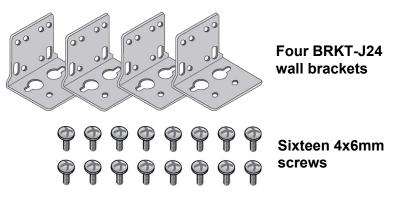


Figure 22. BRKT-J24 Wall Brackets Kit for the x330-20GTX and x330-28GTX Switches

Note

The x330-52GTX Switch comes with brackets for installing the device on a wall.

Recording the Serial Number and MAC Address

The serial number and MAC address of the switch are located on labels on the bottom panel. Refer to Figure 23. If you need to record the numbers for your records, you should do so before installing the device.

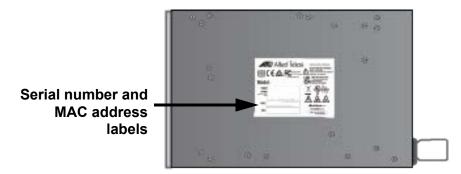


Figure 23. Serial Number and MAC Address Labels

Note

You can also view the serial number and MAC address of the switch with the SHOW SYSTEM SERIALNUMBER and SHOW SYSTEM MAC commands in the User Exec and Privileged EXEC modes of the AlliedWare Plus management software.

Installing the Switch on a Table

You can operate the x330 Switches on a table or desktop. Refer to Figure 24.




Figure 24. x330 Switches Installation on a Table

The following guidelines are in addition to those in "Choosing a Site for the Switch" on page 46:

- Do not stack switches on a table.
- Do not install switches upside down on a table.
- Do not install switches vertically on a table.

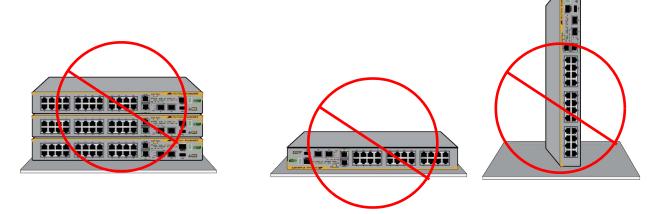


Figure 25. Unsupported Table Installations



Warning

Switches should not be stacked on a table or desktop. They could present a physical safety hazard should you move or replace switches. \sim E91



Warning

The device is heavy. Use both hands to lift it. You might injure yourself or damage the device if you drop it. \mathcal{A} E94

The illustrations in the procedure show the x330-28GTX Switch. The procedure is the same for all x330 Switches.

Note

Bumper feet are required for tabletop installation. They promote cooling by allowing airflow beneath the switch.

To install the switch on a table, perform the following procedure:

- 1. Verify that the selected site is suitable for the unit by reviewing "Reviewing Safety Precautions" on page 42 and "Choosing a Site for the Switch" on page 46.
- 2. Verify that the table is strong enough to support the weight of the switch.
- 3. Verify that the accessory kit came with all the appropriate items. Refer to "Unpacking the Switch" on page 48.
- 4. Lift the switch from the shipping box and place it upside down on the table.
- For the x330-10GTX, x330-20GTX, and x330-28GTX Switches, attach the four bumper feet to the bottom corners of the switch using the four 3x4.5mm screws and a Phillips-head screwdriver. Refer to Figure 26.

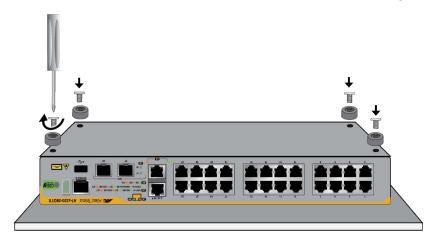


Figure 26. Attaching Bumper Feet on x330-10GTX, x330-20GTX, and x330-28GTX Switches

- 6. For the x330-52GTX Switch, do the following:
 - a. Place a bumper foot over one of the corner holes on the bottom panel of the switch. Refer to Figure 27 on page 61.
 - b. Insert a rivet to secure the bumper foot.

c. Repeat this step to install the remaining bumper feet.



Figure 27. Attaching Bumper Feet on the x330-52GTX Switch

- 7. Turn the switch over, placing it on the bumper feet.
- 8. Go to Chapter 9, "Verifying the Switch" on page 105.

Chapter 2: Beginning the Installation

Chapter 3 Installing the x330-10GTX Switch in an Equipment Rack

The instructions in this chapter explain how to install the x330-10GTX switch in a standard 19-inch equipment rack with the optional RKMT-J05 equipment rack brackets kit. Here are the sections:

- □ "Introduction" on page 64
- □ "Installing the x330-10GTX Switch" on page 66

Introduction

Installing the x330-10GTX switch in a standard 19-inch equipment rack requires the RKMT-J05 equipment rack brackets kit. The brackets allow you to install the switch with the front panel flush with the front of the equipment rack or with the switch projecting in front of the rack. Refer to Figure 28. The kit is sold separately.


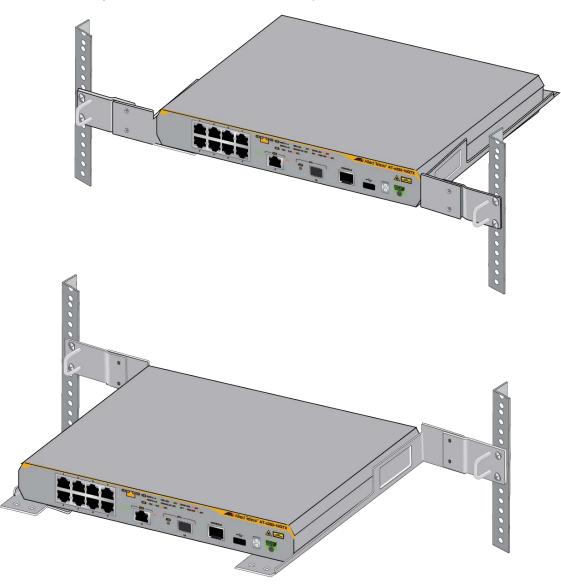


Figure 28. x330-10GTX Switch in an Equipment Rack with the RKMT-J05 Brackets Kit

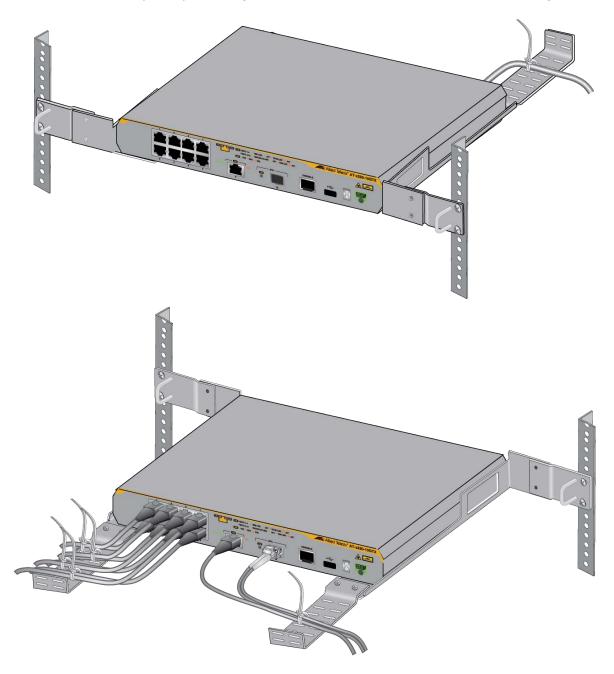

The RKMT-J05 bracket kit includes two cable trays and ten tie wraps for physically securing the power cord or network cables. Refer to Figure 29.

Figure 29. x330-10GTX Switch with RKMT-J05 Cable Trays

Installing the x330-10GTX Switch

This section contains instructions for installing the x330-10GTX switch in a standard 19-inch equipment rack with the optional RKMT-J05 equipment rack brackets kit. Here are the required items:

- □ One RKMT-J05 rack mount brackets kit (sold separately)
- □ Phillips-head screwdriver (not provided)
- □ Four standard equipment rack screws (not provided)

To install the switch in a 19-inch equipment rack with the RKMT-J05 equipment rack brackets kit, perform the following procedure:

1. Place the switch on a table.

Note

If the bumper feet are installed on the bottom panel of the switch, remove them before continuing.

- 2. Unpack the RKMT-J05 equipment rack brackets kit and verify the contents. Refer to Figure 19 on page 55.
- Attach the handles in the RKMT-J05 kit to the short brackets using the supplied M3x6mm pan head screws and a Phillips-head screwdriver. Be sure to attach the handles to the correct sides of the short brackets for your switch-brackets configuration. Refer to Figure 30. The handles are optional.




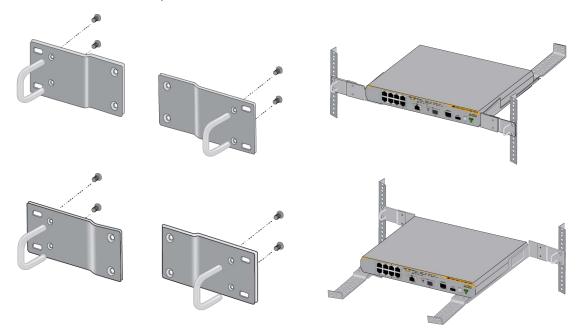


Figure 30. Attaching the RKMT-J05 Handles to the Short Brackets

4. Attach the short brackets to the long brackets using the supplied M4x6mm counter sunk screws. Refer to Figure 31.

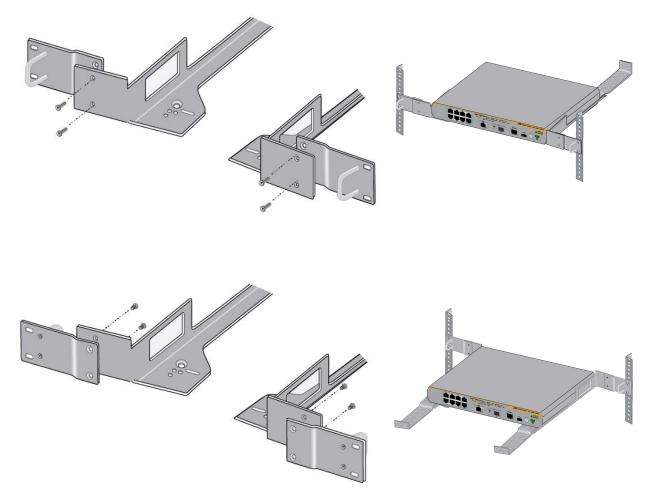



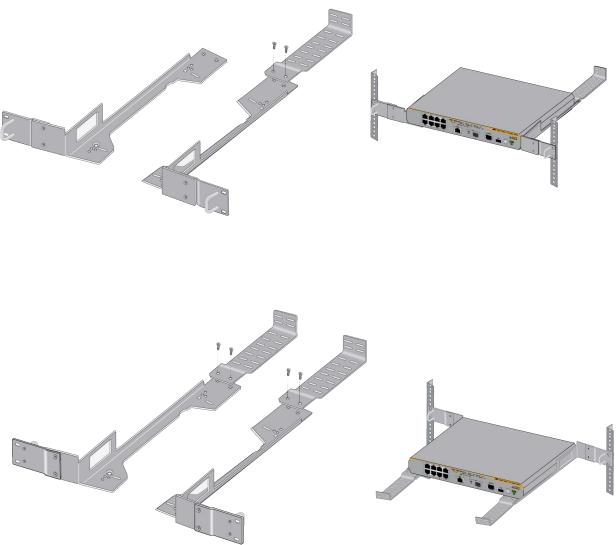

5. Attach one or both cord trays to the long brackets. The cord trays are optional. Refer to Figure 32.

Figure 32. Attaching the RKMT-J05 Cord Trays to the Long Brackets

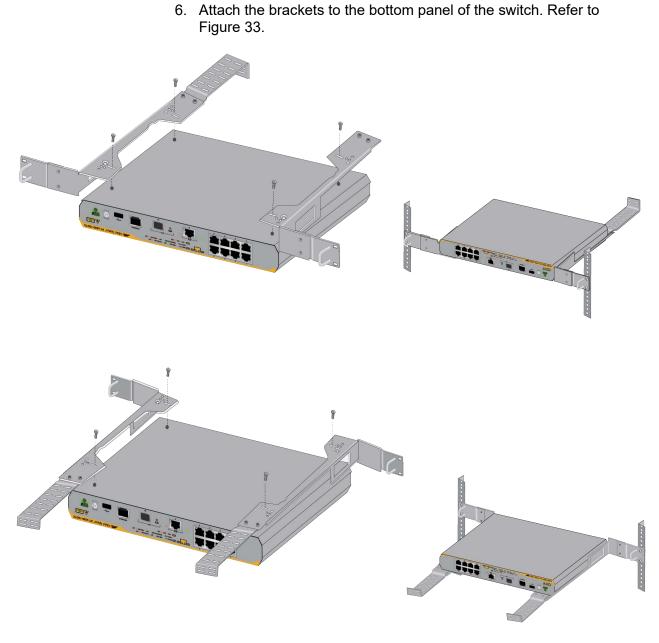


Figure 33. Attaching the RKMT-J05 Brackets to the Switch

7. Turn the switch right-side up on the table.

8. Have another person hold the switch in the equipment rack while you secure it with four standard equipment rack screws (not provided). Refer to Figure 34.

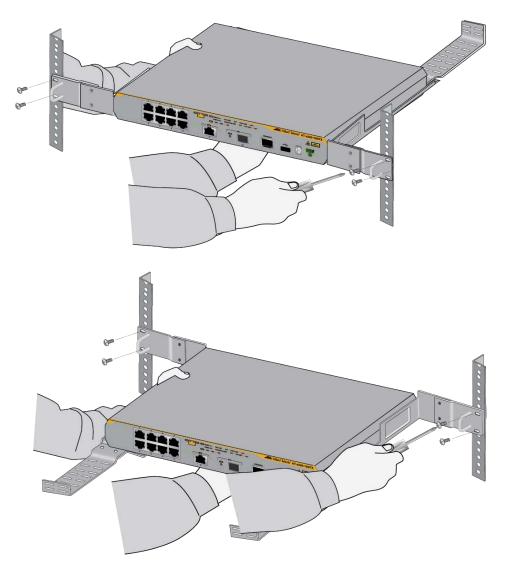


Figure 34. Attaching the x330-10GTX Switch to the Equipment Rack

9. Go to Chapter 9, "Verifying the Switch" on page 105.

Chapter 4 Installing the x330-20GTX Switch in an Equipment Rack

This chapter contains installation instructions for the x330-20GTX Switch in a standard 19-inch equipment rack with the RKMT-J13 equipment rack brackets kit. Here are the sections in the chapter:

- □ "Introduction" on page 72
- □ "Installing the x330-20GTX Switch" on page 73

Introduction

Installing the x330-20GTX Switch in a standard 19-inch equipment rack requires the RKMT-J13 equipment rack brackets kit. The kit allows you to install the switch with its front panel flush with or recessed 50mm (2 in.) behind the front of the equipment rack. Refer to Figure 35. The kit is sold separately.

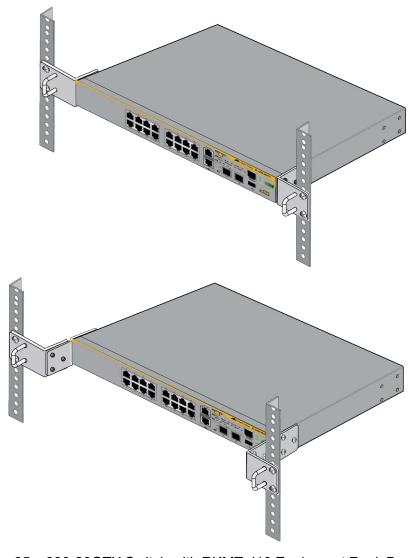


Figure 35. x330-20GTX Switch with RKMT-J13 Equipment Rack Brackets Kit

Note

The x330-28GTX Switch comes with two equipment rack brackets. You can install the switch in an equipment rack with the two brackets included with the unit, or the RKMT-J13 kit.

Installing the x330-20GTX Switch

This section contains the procedure for installing the x330-20GTX Switch in standard 19-inch equipment rack with the RKMT-J13 equipment rack brackets kit. Here are the required items:

- □ One RKMT-J13 equipment rack brackets kit.
- Cross-head screwdriver (not provided).
- □ Flat-head screwdriver (not provided).
- □ Four standard equipment rack screws (not provided).

To install the x330-20GTX Switch in a 19-inch equipment rack, perform the following procedure:

1. Place the switch on a table.

Note

If the bumper feet are installed on the bottom panel of the switch, remove them before continuing.

- 2. Unpack the RKMT-J13 equipment rack brackets kit and verify its contents. Refer to Figure 21 on page 56.
- Attach the handles to the RKMT-J13 brackets with the four 3x6mm screws included in the kit. Attaching the handles is optional. Refer to Figure 36.




Figure 36. Attaching the Handles to the RKMT-J13 Brackets

4. If you want to recess the front of the switch in the equipment rack 50mm (2 in.), attach the extenders to the brackets with six 4x8mm screws included in the kit. Refer to Figure 37 on page 74.

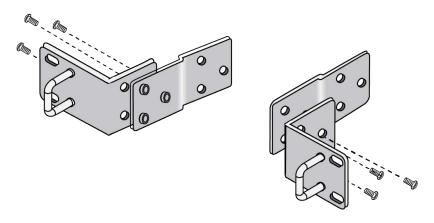


Figure 37. Attaching the Extenders to the RKMT-J13 Brackets

5. Attach the brackets to the sides of the switch with six 4x8mm screws included in the kit. Refer to Figure 38.

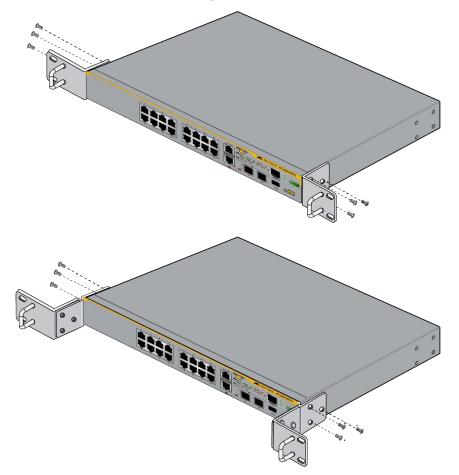


Figure 38. Attaching the RKMT-J13 Brackets to the x330-20GTX Switch

6. Have another person hold the switch at the selected location in the equipment rack while you secure it using four standard equipment rack screws (not provided). Refer to Figure 39.

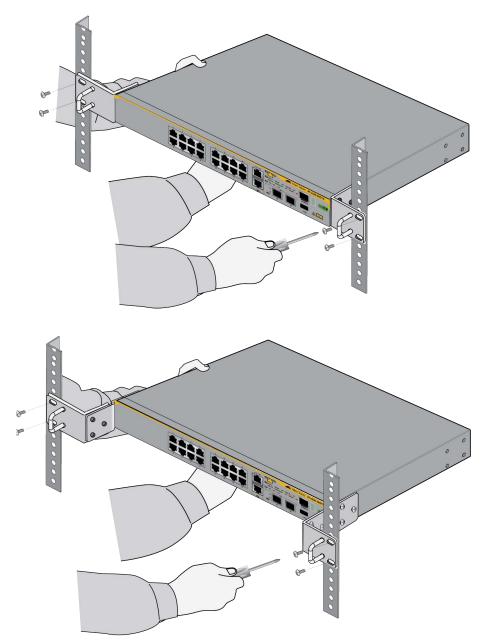


Figure 39. Securing the x330-20GTX Switch in a Standard 19-inch Equipment Rack

7. Go to Chapter 9, "Verifying the Switch" on page 105.

Chapter 4: Installing the x330-20GTX Switch in an Equipment Rack

Chapter 5 Installing the x330-28GTX Switch in an Equipment Rack

This chapter contains the installation instructions for the x330-28GTX Switch in a standard 19-inch equipment rack. Here are the sections:

- □ "Introduction" on page 78
- □ "Installing the x330-28GTX Switch" on page 79

Introduction

The x330-28GTX Switch come with two brackets for installing the devices in standard 19-inch equipment racks. Refer to Figure 40. The brackets and screws are shown in Figure 13 on page 49.

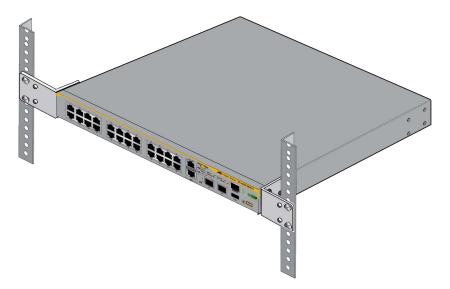


Figure 40. x330-28GTX Switch in Standard 19-inch Equipment Racks

Note

You can install the x330-28GTX Switch in an equipment rack with the brackets that come with the unit or with the RKMT-J13 equipment rack brackets kit, The kit is sold separately.

Installing the x330-28GTX Switch

This section contains the procedure for installing the x330-28GTX Switch in a standard 19-inch equipment rack with the two equipment rack brackets included with the device. Here are the required items:

- □ Two equipment rack brackets (included with the switch).
- □ Six M4x8mm bracket screws (included with the switch).
- □ Cross-head screwdriver (not provided).
- □ Four standard equipment rack screws (not provided).

To install the switch in a 19-inch equipment rack, perform the following procedure:

1. Place the switch on a table.

Note

If the bumper feet are installed on the bottom panel of the switch, remove them before continuing.

2. Attach the equipment rack brackets to the sides of the switch with the six 4x8mm screws included with the device. The brackets can be installed on the switch only one way. Refer to Figure 41.

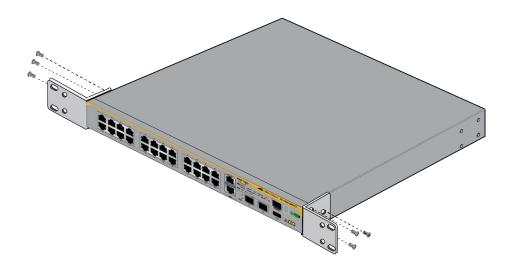


Figure 41. Attaching the Equipment Rack Brackets to the x330-28GTX Switch

3. Have another person hold the switch at the selected location in the equipment rack while you secure it with four standard equipment rack screws (not provided). Refer to Figure 42 on page 80.

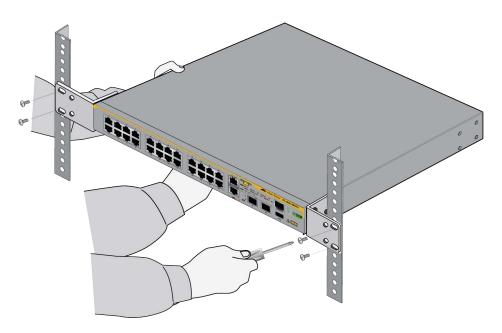


Figure 42. Securing the x330-28GTX Switch in a Standard 19-inch Equipment Rack

4. Go to Chapter 9, "Verifying the Switch" on page 105.

Chapter 6 Installing the x330-52GTX Switch in an Equipment Rack

This chapter contains the installation instructions for the x330-52GTX Switch in a standard 19-inch equipment rack. Here are the sections:

- □ "Introduction" on page 82
- □ "Installing the x330-52GTX Switch" on page 83

Introduction

The x330-52GTX Switch comes with two brackets and eight screws for installing the device in a standard 19-inch equipment rack. Refer to Figure 14 on page 50.

The switch has two sets of four screw holes on the left and right sides for the brackets. Refer to Figure 43.

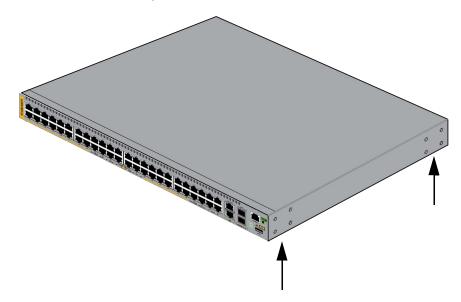


Figure 43. Bracket Screw Holes on the x330-52GTX Switch

You can install the brackets so that the front of the switch is flush with or extending in front of the equipment rack. Refer to Figure 44.

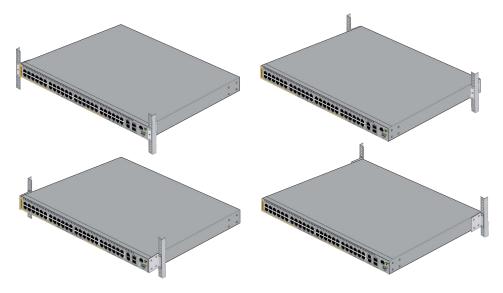


Figure 44. Equipment Rack Bracket Positions for the x330-52GTX Switch

Installing the x330-52GTX Switch

This section contains the procedure for installing the x330-52GTX Switch in a standard 19-inch equipment rack. Here are the required items:

- Two wall/equipment rack brackets (included with the switch).
- Eight M4x8mm bracket screws (included with the switch).
- Cross-head screwdriver (not provided).
- □ Four standard equipment rack screws (not provided).



Warning

The device is heavy. Ask for assistance before moving or lifting it to avoid injuring yourself or damaging the equipment. & E94

To install the switch in a 19-inch equipment rack, perform the following procedure:

1. Place the switch on a table.

Note

If the bumper feet are attached to the bottom of the switch, remove them with a flathead screwdriver before continuing.

2. Attach the wall/equipment rack brackets to the sides of the switch in the selected position, with the eight 4x8mm screws included with the switch. Figure 45 shows the brackets installed so that the front of the switch is flush with the front of the equipment rack.

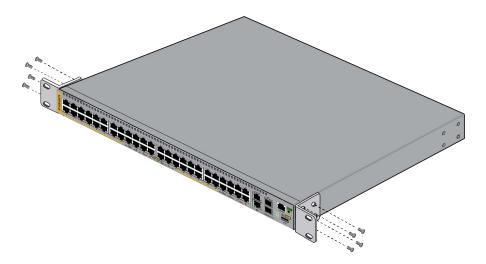


Figure 45. Attaching the Equipment Rack Brackets to the x330-52GTX Switch

3. Have another person hold the switch at the selected location in the equipment rack while you secure it using four standard equipment rack screws (not provided). Refer to Figure 46.

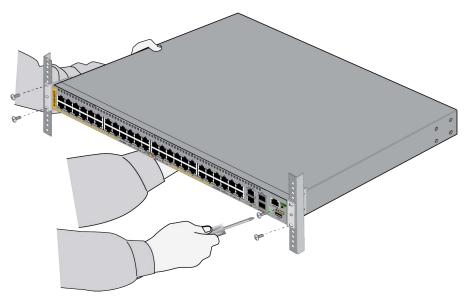


Figure 46. Securing the x330-52GTX Switch in a Standard 19-inch Equipment Rack

4. Go to Chapter 9, "Verifying the Switch" on page 105.

Chapter 7 Installing the x330-10GTX Switch on a Wall

This chapter explains how to install the x330-10GTX Switch on a wall with the BRKT-J23 wall brackets kit. The sections are listed here:

- □ "Introduction" on page 86
- □ "Installation Guidelines" on page 88
- □ "Installing the x330-10GTX Switch" on page 89

Introduction

Installing the x330-10GTX Switch on a wall requires the BRKT-J23 wall bracket kit. The kit contains two identical brackets. Refer to Figure 20 on page 56. The BRKT-J23 bracket kit is sold separately.

You can install the switch with the front panel facing up, left or right, with two or four brackets. Figure 47 shows the switch with two brackets.

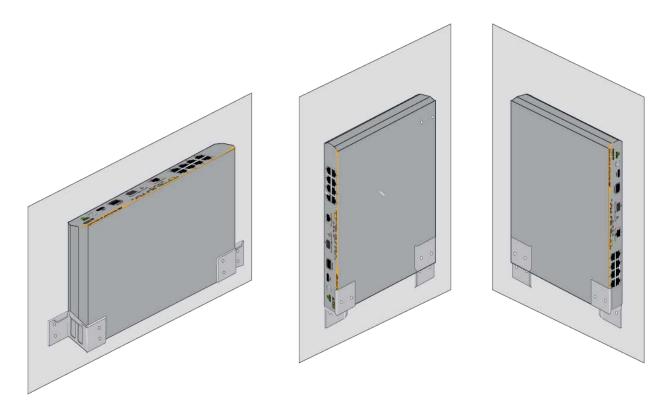


Figure 47. x330-10GTX Switch with Two BRKT-J23 Wall Brackets

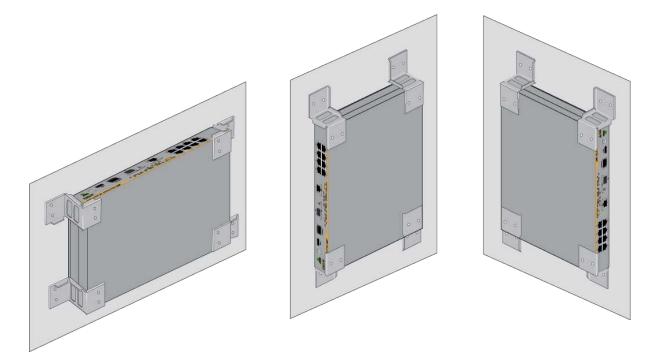


Figure 48 shows the switch with four brackets.

Figure 48. x330-10GTX Switch with Four BRKT-J23 Wall Brackets

Do not install the switch with the front panel facing down. Refer to Figure 49.

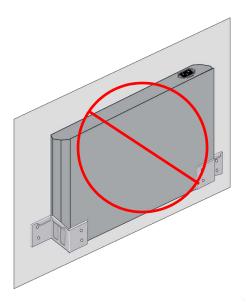


Figure 49. Unsupported Wall Installation with Front Panel Facing Down

Installation Guidelines

Here are the guidelines to installing the switch on a wall:

- As shown in Figure 47 on page 86 and Figure 48 on page 87, the BRKT-J23 brackets secure the device by its sides. Installing the brackets over the front or rear panel will block copper ports or the AC power connector.
- Installing the switch with two brackets requires one BRKT-J23 bracket kit. Installing the switch with four brackets requires two BRKT-J23 bracket kits.
- □ You can install the switch on a wooden or concrete wall.
- □ The BRKT-J23 bracket kit does not include wall screws or anchors.
- **The diameter of the screw holes in the brackets is 4mm.**
- You should not install the switch only on sheetrock or similar material. Sheetrock might not be strong enough to safely support the device.



Warning

The device should be installed on a wall by a qualified building contractor. Serious injury to yourself or others or damage to the equipment may result if it is not properly fastened to the wall. \mathcal{C} E105



Warning

The device is heavy. Use both hands to lift it. You might injure yourself or damage the device if you drop it. Ger E94

Installing the x330-10GTX Switch

Here are the required tools and material for installing the switch on a wooden or concrete wall with the BRKT-J23 brackets:

- One or two BRKT-J23 bracket kits
- □ Four or eight wall screws (not provided)
- □ Cross-head screwdriver (not provided)
- Stud finder for a wooden wall, capable of identifying the middle of wall studs and hot electrical wiring (not provided)

Depending on the wall material these items might also be required:

- Drill for pre-drilling the holes (not provided)
- □ Four or eight wall anchors (not provided)



Caution

The supplied screws and anchors may not be appropriate for all wall material. A qualified building contractor should determine the appropriate hardware requirements for your wall before installing the switch. \swarrow E88

Please review "Reviewing Safety Precautions" on page 42 and "Choosing a Site for the Switch" on page 46 before performing this procedure. This procedure requires two people.



Warning

The device is heavy. Use both hands to lift it. You might injure yourself or damage the device if you drop it. Ger E94



Warning

The device should be installed on the wall by a qualified building contractor. Serious injury to yourself or others or damage to the equipment may result if it is not properly fastened to the wall. 65 E105

Depending on the selected wall location for the switch, it may be easier to verify the switch and connect the cables to the ports before mounting the device on the wall. If this is true for your installation, perform the procedures in Chapter 9, "Verifying the Switch" on page 105 and Chapter 10, "Cabling Copper and SFP+ Ports" on page 117 before performing this procedure.

To install the x330-10GTX Switch on a wall, perform the following procedure:

1. Place the switch on a table.

Note

If the bumper feet are installed on the bottom panel of the switch, remove them before continuing.

- 2. Unpack the BRKT-J23 wall brackets kit and verify the contents. Refer to Figure 20 on page 56.
- 3. Have another person hold the switch on the wall at the selected location and orientation. Be sure to leave sufficient space from other devices or walls so that you can access the front and back panels.
- 4. Position the brackets on the wall and mark the bracket screw holes. Refer to Figure 50 and Figure 51 on page 91.

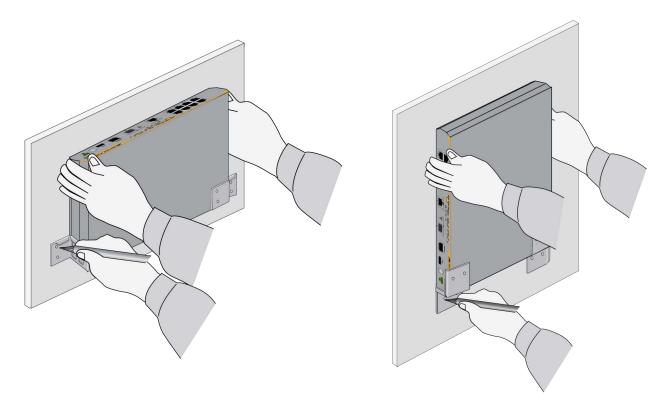


Figure 50. Marking the Screw Holes for Two BRKT-J23 Brackets

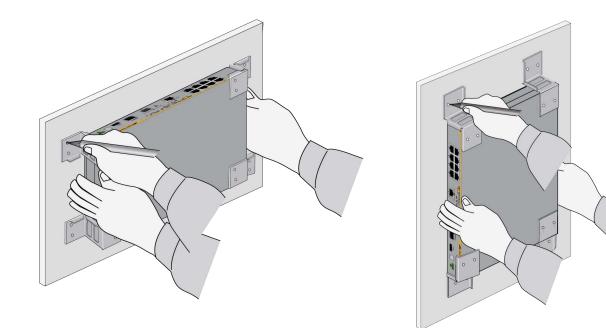


Figure 51. Marking the Screw Holes for Four BRKT-J23 Brackets

- 5. Place the switch and brackets on a table.
- 6. For a wooden wall, use a stud-finder to determine if there are any live electrical wires at the screw hole locations.
- 7. If required, pre-drill the screw holes on the wall. For a concrete wall, observe the following:
 - □ Set the drill to hammer and rotation mode to break up the concrete and clean out the hole.
 - □ Clean out the holes with a brush or compressed air.
- 8. If required, install wall anchors.
- 9. Attach the bottom BRKT-J23 brackets to the wall with appropriate screws. Refer to Figure 52 on page 92.



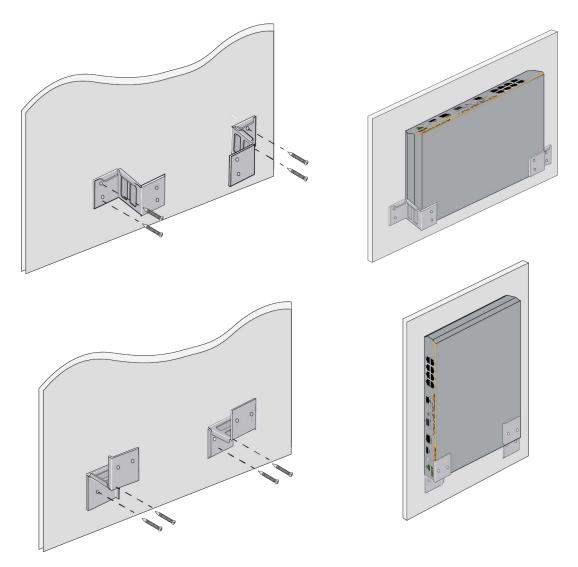


Figure 52. Attaching the Bottom BRKT-J23 Brackets to the Wall


10. Slide the switch into the BRKT-J23 brackets. Refer to Figure 53.

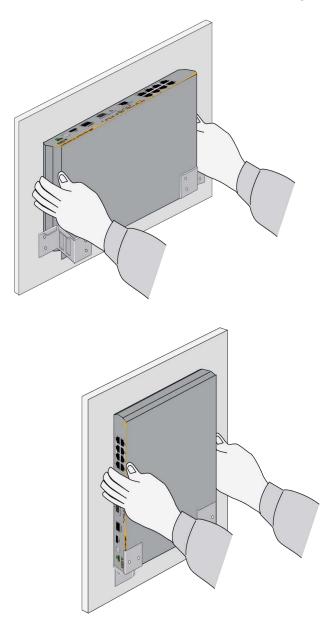



Note

If you are installing the switch with two brackets, skip the next step and go to Chapter 9, "Verifying the Switch" on page 105. If you are installing the switch with four brackets, continue with the next step.

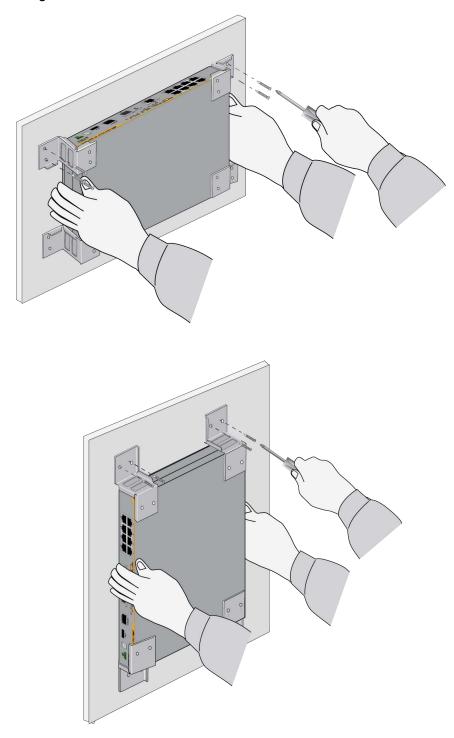

11. Attach the two top brackets to the wall with appropriate screws. Refer to Figure 54.

Figure 54. Attaching the Top BRKT-J23 Brackets to the Wall 12. Go to Chapter 9, "Verifying the Switch" on page 105.

Chapter 8 Installing x330-20GTX, x330-28GTX, and x330-52GTX Switches on a Wall

This chapter contains instructions for installing x330-20GTX, x330-28GTX, and x330-52GTX Switches on a wood or concrete wall. The chapter contains the following sections:

- □ "Installation Guidelines" on page 96
- □ "Plywood Base for a Wall with Wooden Studs" on page 99
- □ "Installing the Switch" on page 101

Installation Guidelines

The guidelines to installing x330-20GTX, x330-28GTX, and x330-52GTX Switches on a wall are listed here:

- The x330-20GTX and x330-28GTX Switches require the AT-BRKT-J24 brackets kit for wall installations. The kit comes with four identical brackets. Refer to Figure 22 on page 57. The kit is sold separately.
- The x330-52GTX Switch is installed on a wall with the two wall/ equipment rack brackets included with the unit. Refer to Figure 14 on page 50.
- ☐ You can install the switches on walls with the front panels facing up, left or right. Refer to Figure 55 and Figure 56.

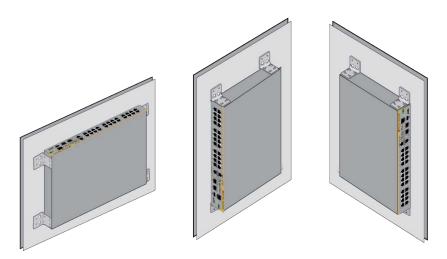


Figure 55. x330-20GTX and x330-28GTX Switches on a Wall with the AT-BRKT-J24 Brackets Kit

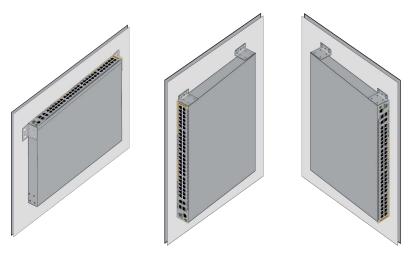


Figure 56. x330-52GTX Switch on a Wall

Do not install switches with the front panels facing down. Refer to Figure 57.




Figure 57. Unsupported Wall Installation for the x330-20GTX, x330-28GTX, and x330-52GTX Switches

- □ You may install the switches on wooden or concrete walls.
- If you are installing the switches on a wall with wooden studs, you should install them on a plywood base. For more information, refer to "Plywood Base for a Wall with Wooden Studs" on page 99.
- You should not install the switches on a wall that has metal studs. Metal studs may not be strong enough to safely support the device.
- You should not install the switches on sheetrock or similar material. Sheetrock might not be strong enough to safely support the devices.
- □ Attach the base to two wall studs with a minimum of four screws.
- The selected wall location should provide sufficient space from other devices or walls so that you can access the front and back panels, and for adequate air flow for ventilation.
- □ For wooden walls, use a stud finder to identify the middle of studs and hot electrical wiring.



Warning

The device is heavy. Ask for assistance before moving or lifting it to avoid injuring yourself or damaging the equipment. & E94



Warning


The device should be installed on a wall by a qualified building contractor. Serious injury to yourself or others or damage to the equipment may result if it is improperly fastened to the wall. & E105


Here are the required tools and material for installing the switch on a wall:

- □ For x330-20GTX and x330-28GTX Switches, one AT-BRKT-J24 wall brackets kit for each switch. The kit is sold separately.
- □ For the x330-52GTX Switch, two wall//equipment rack brackets are included with the device.
- □ Four wall anchors and screws (not provided) The diameter of the screw holes in the brackets is 5mm.
- Cross-head screwdriver (not provided).
- Stud finder for a wooden wall, capable of identifying the middle of wall studs and hot electrical wiring (not provided).
- Drill and 1/4-inch carbide drill bit for a concrete wall (not provided).
- Plywood base if you are installing the switch on a wall with wooden studs (not provided.) Refer to "Plywood Base for a Wall with Wooden Studs" on page 99 for illustrations.
- Four screws for attaching the plywood base to the wall (not provided).

Plywood Base for a Wall with Wooden Studs

When installing a switch on a wall that has wooden studs, Allied Telesis recommends installing it on a plywood base. (A plywood base is not required for concrete walls.) Refer to Figure 58.

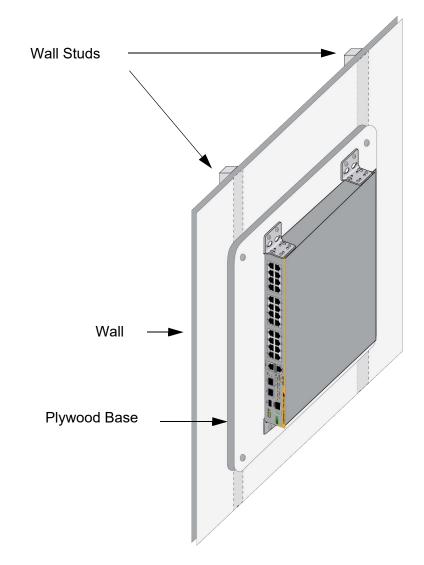



The plywood base should be mounted on two studs in the wall. Recommended minimum dimensions of a plywood base for the x330-20GTX and x330-28GTX Switches are listed here:


- □ Width: 55.9 centimeters (22 inches)
- □ Height: 50 centimeters (20 inches)
- □ Thickness: 2.5 centimeters (1 inch)

Recommended minimum dimensions of a plywood base for the x330-52GTX Switch are listed here:

- □ Width: 55.9 centimeters (22 inches)
- □ Height: 50 centimeters (22 inches)
- □ Thickness: 2.5 centimeters (1 inch)

The dimensions assume the wall studs are 41 centimeters (16 inches) apart. You might need to adjust the width of the base if the distance between the studs in your wall differs from the industry standard.

You should install the plywood base on the wall and then install the switch on the base. Refer to Figure 59.

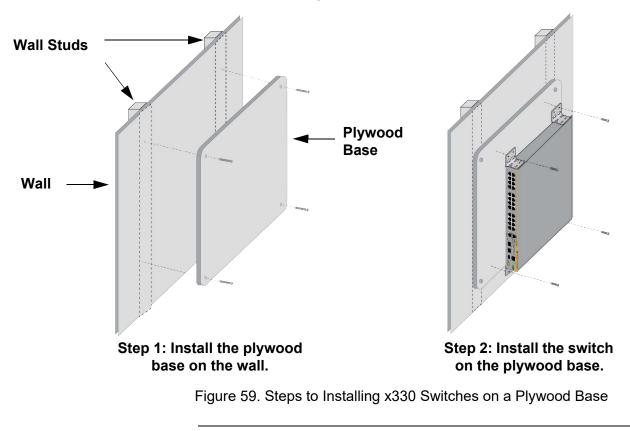

Note

Consult a qualified building contractor for installation instructions for the plywood base.

Installing the Switch

This section contains the procedure for installing the switch on a wall. Review the following before performing the procedure:

- If you are installing the switch on a wall with wooden studs, the procedure assumes the plywood base is already mounted on the wall.
- Review "Reviewing Safety Precautions" on page 42 and "Choosing a Site for the Switch" on page 46 before performing this procedure.
- Allied Telesis recommends a minimum of two people for this procedure.



Warning

The device is heavy. Always ask for assistance before moving or lifting it to avoid injuring yourself or damaging the equipment.



Warning

The device should be installed on the wall by a qualified building contractor. Serious injury to yourself or others or damage to the equipment may result if it is improperly fastened to the wall. & E105

To install the switch on the wall, perform the following procedure:

1. Place the switch on a table.

Note

If the bumper feet are attached to the bottom on the switch, remove them before continuing.

 For x330-20GTX and x330-28GTX Switches, attach the four AT-BRKT-J24 wall brackets to the sides of the switch, with the sixteen M4x6mm screws included in the brackets kit. Refer to Figure 60 on page 102.

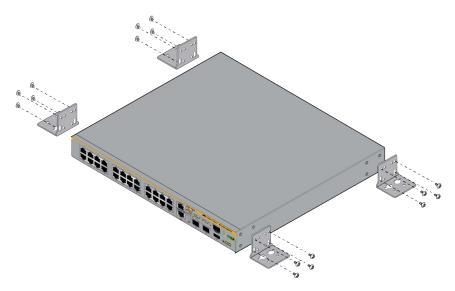


Figure 60. Attaching the AT-BRKT-J24 Wall Brackets to x330-20GTX and x330-28GTX Switches

3. For the x330-52GTX Switch, attach the two wall/equipment rack brackets to one side of the switch. Refer to Figure 61 and Figure 62 on page 103 for the bracket positions.

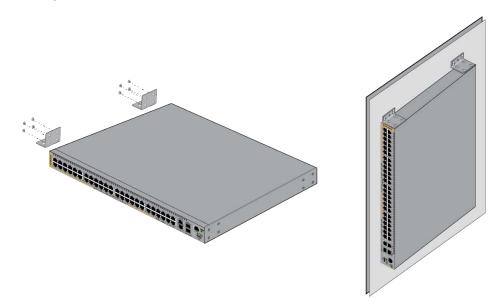


Figure 61. Attaching the Wall/Equipment Rack Brackets to the x330-52GTX Switch

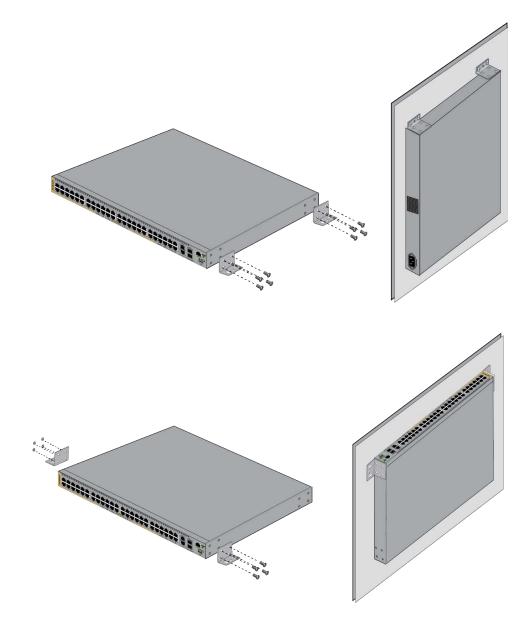


Figure 62. Attaching the Wall/Equipment Rack Brackets to the x330-52GTX Switch (continued)

Note

If the wall requires pre-drilled holes, such as a concrete wall, continue with the next step. Otherwise, go to step 8.

4. Have another person hold the switch on the wall at the selected location for the device while you use a pencil or pen to mark the wall with the locations of the screw holes in the brackets. Refer to Figure 63 on page 104.

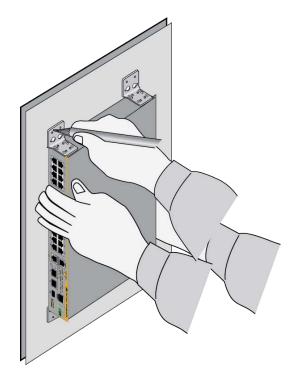


Figure 63. Marking the Locations of the Bracket Holes

- 5. Place the switch on a table or desk.
- 6. Use a drill and appropriate drill bit, such as a 1/4" carbide drill for concrete walls, to pre-drill the holes you marked in the step 4. Review the following guidelines:
 - □ For concrete walls, set the drill to hammer and rotation mode. The modes break up the concrete and clean out the hole.
 - □ Allied Telesis recommends cleaning out the holes with a brush or compressed air.
- 7. If the wall material requires anchors, insert appropriate anchors in the holes.
- 8. Have another person hold the switch on the wall while you secure it with appropriate screws.
- 9. Go to Chapter 9, "Verifying the Switch" on page 105.

Chapter 9 Verifying the Switch

The procedures in this chapter explain how to start a local management session on the switch, verify its hardware status, and disable the VCStack feature to use the switch as a standalone device. This chapter contains the following procedures:

- □ "Powering On the Switch" on page 106
- □ "Starting a Management Session" on page 108
- □ "Displaying the Hardware Status and Disabling VCStack" on page 113

Powering On the Switch

For AC power specifications, refer to "Power Specifications" on page 135.



Warning Power cord is used as a disconnection device. To de-energize

equipment, disconnect the power cord. $\ensuremath{\textup{eq}}$ E3

Note

Pluggable Equipment. The socket outlet shall be installed near the equipment and shall be easily accessible. & E5

To power on the switch, perform the following procedure:

1. Install the power cord retaining clip on the AC power connector on the rear panel of the switch, as shown in Figure 64.

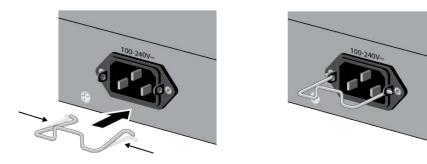


Figure 64. Installing the Power Cord Retaining Clip

2. Raise the retaining clip and connect the AC power cord to the AC power connector on the rear panel. Refer to Figure 65.





Figure 65. Connecting the AC Power Cord

3. Lower the power cord retaining clip to secure the cord to the switch. Refer to Figure 66.




Figure 66. Lowering the Power Cord Retaining Clip

4. Connect the power cord to an appropriate AC power source. Refer to Figure 67.




Figure 67. Connecting the Power Cord to an AC Power Source

Note

The illustration shows a North American power cord. Your power cord may be different.

- 5. Wait one minute for the switch to start the AlliedWare Plus management software.
- 6. Go to "Starting a Management Session" on page 108.

Starting a Management Session

The following procedures explain the different methods for starting the first management session on the switch:

- □ "Through the Console Port," next
- □ "With a DHCP or DHCPv6 Server" on page 110
- □ "Without a DHCP or DHCPv6 Server" on page 111

Through the
Console PortThis section explains how to start a local management session through
the Console port on the switch. This procedure requires a terminal,
computer, or laptop with an RS-232 DB-9 serial port or USB port, and a
terminal emulator, such as PuTTy. Here are the guidelines:

Local management sessions require a management cable. If your computer has an RS-232 port, you can use the management cable supplied with the product, shown in Figure 68. The cable has a RJ-45 connector that connects to the Console port on the switch, and a female DB-9 (D-sub 9-pin) connector that connects to your computer.



Figure 68. Management Cable Included with Switch

If your computer has a USB port, you may need to purchase a USB-to-Serial converter that is compatible with its operating system. An example is the VT-Kit3 converter from Allied Telesis, shown in Figure 69. The VT-Kit3 converter is sold separately.





Local management sessions do not interfere with the network operations of the switch. The switch does not need an IP address for local management sessions.

To start a local management session, perform the following procedure:

- 1. Power on the switch and wait several minutes for it to initialize the AlliedWare Plus management software.
- 2. Connect your computer to the Console port on the switch:
 - If your computer has an RS-232 port, connect the DB-9 connector on the supplied management cable to a DB-9 port on your computer or terminal, and the cable's RJ-45 connector to the Console port on the switch.
 - If your computer has a USB port, use a USB-to-Serial converter. To use the VT-Kit3 from Allied Telesis, connect the USB connector on the VT-Kit3 to a USB port on your computer or terminal. To connect the kit to the Console port on the switch, use a standard, straight-through Ethernet cable. Refer to Figure 70.



Figure 70. Local Management with the VT-Kit3 Management Cable

- 3. Configure the VT-100 terminal or terminal emulation program:
 - Baud rate: 9600 bps (The baud rate of the Console port is adjustable from 1200 to 115200 bps. The default is 9600 bps.)
 - Data bits: 8
 - Parity: None
 - □ Stop bits: 1
 - □ Flow controller: None

Note

The port settings are for a DEC VT100 or ANSI terminal, or an equivalent terminal emulator program.

Note

The baud rate must be set to the default 9600 bps to configure the boot loader.

- 4. Press Enter. You are prompted for the name and password of the manager account.
- 5. Enter the default user name "manager" and password "friend", without the quotes.

Note

User names and passwords are case sensitive.

The switch starts the local management session and displays the following prompt:

awplus>

The prompt is the User Exec mode of the command line interface.

6. Go to "Displaying the Hardware Status and Disabling VCStack" on page 113.

With a DHCP or DHCPv6 Server

This section contains the procedure for starting the first management session with the switch on a network that has a DHCP or DHCPv6 server. Review the following factory default settings for the switch when powered on for the first time:

- DHCP and DHCPv6 clients: enabled
- □ SSH server: enabled
- Telnet server: disabled
- Web server: enabled
- □ Switch ports: enabled
- VLAN membership: port-based VLAN1
- Configuration file: none (The switch creates a configuration file the first time you save the parameter settings.)

To start a management session on the switch over a network that has a DHCP or DHCPv6 server, perform the following procedure:

- Enter the MAC address of the switch into your DHCP or DHCPv6 server so that the server assigns it an address when you power it on. The MAC address label is on the bottom panel of the switch, as shown in "Recording the Serial Number and MAC Address" on page 58. Refer to your DHCP server's documentation for instructions.
- 2. Connect a single Ethernet port on the switch to your existing network.
- 3. Power on the switch and wait several minutes for it to initialize the AlliedWare Plus management software and obtain its IPv4 or IPv6 address from the existing DHCP server.
- 4. On your management workstation, enter the switch's assigned IP address into a Secure Shell (SSH) application or the URL field of your web browser on your workstation.
- 5. Press Enter. You are prompted for the name and password of the manager account.
- 6. Enter the default user name "manager" and password "friend", without the quotes.

Note

User names and passwords are case sensitive.

The switch starts the local management session and displays the following prompt:

awplus>

The prompt is the User Exec mode of the command line interface.

7. Go to "Displaying the Hardware Status and Disabling VCStack" on page 113.

Without a DHCP or DHCPv6 Server

This section contains the procedure for starting the first management session with the switch on a network without a DHCP or DHCPv6 server. Review the following factory default settings for the switch when powered on for the first time:

- Default IP address (no DHCP server): 169.254.42.42 (255.255.0.0)
- □ SSH server: enabled
- Telnet server: disabled
- □ Web server: enabled
- □ Switch ports: enabled

- □ VLAN membership: port-based VLAN1
- □ Configuration file: none (The switch creates a configuration file the first time you save its parameter settings.)

To start a management session on the switch over a network without a DHCP or DHCPv6 server, perform the following procedure:

- 1. Change the IP address of your workstation to 169.254.42.*n*/16 (255.255.0.0), where *n* is any number from 1 to 254, but not 42.
- 2. Connect the Ethernet port on your workstation to an Ethernet port on the switch.
- 3. Power on the switch and wait several minutes for it to initialize the AlliedWare Plus management software.
- 4. Enter the IP address 169.254.42.42, the switch's default IP address, in an SSH application or the URL field of the web browser on your workstation.
- 5. Press Enter. You are prompted for the name and password of the manager account.
- 6. Enter the default user name "manager" and password "friend", without the quotes.

Note

User names and passwords are case sensitive.

The switch starts the local management session and displays the following prompt:

awplus>

The prompt is the User Exec mode of the command line interface.

7. Go to "Displaying the Hardware Status and Disabling VCStack" on page 113.

Displaying the Hardware Status and Disabling VCStack

This section contains the procedure for verifying the hardware status of the switch from a local or remote management session. It also explains how to disable the VCStack feature so that you can use the switch as a standalone device, with SFP+ ports S1 and S2 as regular Ethernet ports.

Note	
The x330-10GTX Switch does not support the VCStack feature.	

To verify the hardware operations of the switch, perform the following procedure:

- 1. Start a local or remote management session on the switch. Refer to "Starting a Management Session" on page 108.
- 2. Enter the SHOW SYSTEM ENVIRONMENT command in the User Exec or Privileged Exec mode.
- 3. Check the Status column. All components should have the "OK" status.
- 4. Do one of the following:
 - □ For the x330-10GTX Switch, which does not support VCStack, go to Chapter 10, "Cabling Copper and SFP+ Ports" on page 117.
 - □ For all other x330 Switches, continue with the next step to disable VCStack and use the switch as a standalone device.



Caution

You have to reset the switch after disabling the VCStack feature. Some network traffic may be lost if the device is connected to a live network. & E89

5. Enter the ENABLE and CONFIGURE TERMINAL commands to move to the Global Configuration mode. Refer to Figure 71.

```
awplus> enable
awplus# configure terminal
Enter configuration commands, one per line. End with CNTL/Z
awplus(config)#
```

Figure 71. Moving to the Global Configuration Mode

- 6. To. disable the VCStack feature, enter the NO STACK ENABLE command in this format:
- no stack *id* enable

The ID parameter is the ID number of the switch, displayed on the ID LED. Replace the parameter with the number displayed by the ID LED. For example, if the Switch ID LED number is 1, the default value, you enter the command as follows:

```
awplus(config)# no stack 1 enable
```

The confirmation prompt in Figure 72 is displayed.

Warning; This will disable the stacking hardware on member-1. Are you sure you want to continue? (y/n):

Figure 72. Confirmation Prompt for the NO STACK ENABLE Command

- 7. Type Y to disable VCStack on the switch.
- 8. Enter the EXIT command to return to the Privileged Exec mode. Refer to Figure 73.

```
awplus(config)# exit
awplus#
```

Figure 73. Returning to the Privileged Exec Mode

9. Enter the WRITE command to save your change in the configuration file. The switch displays the confirmation prompt in Figure 74.

```
awplus# write
Building configuration ...
[OK]
awplus#
```

Figure 74. Saving the Changes with the WRITE Command

If this is the first management session, the switch creates the Default.cfg file in flash memory to store your changes.

- 10. Enter the REBOOT command to reboot the switch.
- 11. At the confirmation prompt, type "Y" for yes.
- 12. Wait one minute for the switch to start the AlliedWare Plus management software.

13. Examine the Switch ID LED. The ID number should be "0", indicating that VCStack is disabled. The switch is now operating as a standalone unit with the switch ID "1". The S1 and S2 ports are now regular networking ports.

If the Switch ID LED on the front panel is still displaying "1", repeat this procedure, being sure to save the configuration change with the WRITE command in step 9.

14. Go to Chapter 10, "Cabling Copper and SFP+ Ports" on page 117.

Chapter 9: Verifying the Switch

Chapter 10 Cabling Copper and SFP+ Ports

This chapter contains the following sections:

- □ "Cabling Copper Ports" on page 118
- □ "Guidelines to Handling SFP and SFP+ Transceivers" on page 119
- □ "Installing 1Gbps SFP and 10Gbps SFP+ Transceivers" on page 120
- "Installing AT-SP10TW Direct Connect Twinax Cables in SFP+ Ports" on page 123

Cabling Copper Ports

Here are the guidelines to cabling the copper ports:

- □ The cable specifications are in "10/100/1000Mbps Copper Ports" on page 24 and "1/2.5/5/10Gbps Multi-Gigabit Copper Ports" on page 26.
- □ The connectors on the cables should fit snugly into the ports, and the tabs should lock the connectors into place.
- The default speed setting for the ports is Auto-Negotiation. This setting is appropriate for ports connected to network devices that also support Auto-Negotiation.
- Ports must be set to Auto-Negotiation, the default setting, to operate at 1000Mbps and higher speeds.
- □ The ports support full-duplex only at 1000Mbps and higher speeds.
- Do not attach cables to ports of static or LACP port trunks until after configuring the trunks on the switch. Otherwise, the ports might form network loops that can adversely affect network performance.

Guidelines to Handling SFP and SFP+ Transceivers

Please review the following guidelines before installing SFP and SFP+ transceivers in the switches:

- □ Transceivers are hot-swappable. You can install them while the switch is powered on.
- □ For a list of supported transceivers, refer to the product's data sheet on the Allied Telesis web site.
- The operational specifications and fiber optic cable requirements of the transceivers are provided in documents included with the devices.
- You should install a transceiver before connecting its fiber optic cable.
- Fiber optic transceivers are dust sensitive. Always keep the plug in the optical bores when a fiber optic cable is not installed, or when you store the transceiver. When you do remove the plug, keep it for future use.
- Unnecessary removal and insertion of transceivers can lead to their premature failures.



Caution

Transceivers can be damaged by static electricity. Be sure to observe all standard electrostatic discharge (ESD) precautions, such as wearing an anti-static wrist strap, to avoid damaging the devices. & E92

Installing 1Gbps SFP and 10Gbps SFP+ Transceivers

This section contains installation instructions for SFP and SFP+ transceivers. The transceiver in the illustrations has a duplex LC connector. Your transceivers may have different connectors. To install transceivers, perform the following procedure:

- 1. Select an SFP+ port for the transceiver.
- 2. Remove the transceiver from its shipping container and store the packaging material in a safe location.
- 3. Position the transceiver with the Allied Telesis label facing up. Refer to Figure 75.

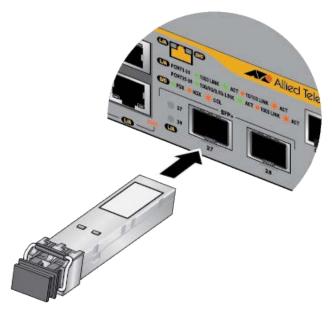


Figure 75. Installing an SFP+ Transceiver

4. Slide the transceiver into the port until it clicks into place.

Note

If you are ready to attach the fiber optic cable to the transceiver, continue with the next step. Otherwise, repeat steps 1 to 4 to install a second transceiver in the switch.

5. Remove the dust cover from the transceiver, as shown in Figure 76 on page 121.




Figure 76. Removing the Dust Cover from an SFP+ Transceiver

6. Verify that the transceiver handle is in the upright position. Refer to Figure 77.

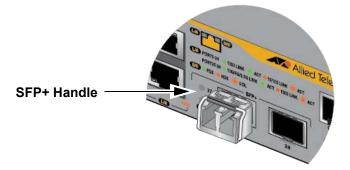


Figure 77. Positioning the SFP+ Handle in the Upright Position

7. Connect the fiber optic cable to the transceiver. Refer to Figure 78 on page 122. The cable connector should fit snugly into the port, and the tab should lock the connector into place.

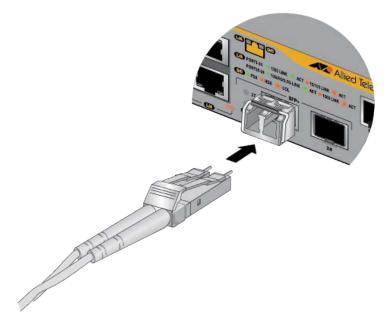


Figure 78. Connecting a Fiber Optic Cable to an SFP or SFP+ Transceiver

8. Repeat this procedure to install a second transceiver.

Note The x330-10GTX Switch has only one SFP+ transceiver port.

Installing AT-SP10TW Direct Connect Twinax Cables in SFP+ Ports

The SFP+ ports support AT-SP10TW1 and AT-SP10TW3 direct connect twinax cables. The cables offer an economical way to add 10Gbps connections over short distances. They have SFP+ transceivers on both ends and come in lengths of one and three meters.

Note The x330 Switches do not support the seven meter AT-SP10TW7 cable.

To install AT-SP10TW cables, perform the following procedure:

- 1. Select an SFP+ port for the transceiver.
- 2. Remove the transceiver from its shipping container and store the packaging material in a safe location.
- 3. Position the transceiver with the Allied Telesis label facing up. Refer to Figure 79.

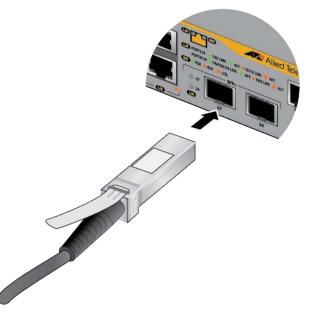


Figure 79. Installing an AT-SP10TW Cable

- 4. Slide the transceiver into the port until it clicks into place.
- 5. Connect the other end of the cable into an SFP+ port on another network device.

6. Repeat this procedure to install a second transceiver.

Note

To remove the connector and cable from the port, gently push on the connector, pull on the release tab, and slide the connector from the switch.

Chapter 11 Troubleshooting

This chapter contains suggestions on troubleshooting problems with the switch.

Note

For further assistance, contact Allied Telesis Technical Support at **www.alliedtelesis.com/us/en/services-support**.

Problem 1: The ports are connected to network devices but the port LEDs and Switch ID LED are off.

Solutions: Try the following:

- Verify that the power cord is securely connected to the power source and the AC connector on the back panel of the switch.
- Verify that the power outlet has power by connecting another device to it.
- **Try connecting the unit to another power source.**
- □ Try a different power cord.
- Verify that the voltage from the power source is within the required levels for your region. The power requirements for the switch are listed in "Power Specifications" on page 135.
- The switch might be operating in the low power eco-friendly mode. To toggle on the LEDs, press the eco-friendly button on the front panel or enter the NO ECOFRIENDLY LED command in the command line interface.

Problem 2: A copper port is connected to an active network device, but the port's link/activity and duplex LEDs are off.

Solutions: The port has not established a link to the network device. Try the following:

- Verify that the network device connected to the copper port is powered on and operating properly.
- Try connecting another network device to the port with a different cable. If the port is able to establish a link, then the problem is with the cable or the other network device.
- Verify that the cable does not exceed 100 meters (328 feet).

- Verify that you are using the appropriate category of cable. Cable requirements are listed in Table 1 on page 24 and Table 2 on page 26.
- □ Verify that the port is connected to the correct cable.

Note

Copper ports may require up to five to ten seconds to establish links to network devices.

Problem 3: The link/activity LED for an SFP or SFP+ transceiver is off.

Solutions: The fiber optic port on the transceiver has not established a link to the remote network device. Try the following:

- Verify that the remote network device connected to the fiber optic port is operating properly.
- Verify that the fiber optic cable is securely connected to the port on the transceiver and to the port on the remote network device.
- Check that the transceiver is fully inserted into the port in the switch.
- Verify that the operating specifications of the fiber optic ports on the transceiver and remote network device are compatible by referring to their documentation.
- □ Verify that the correct type of fiber optic cabling is being used.
- Verify that the port is connected to the correct fiber optic cable.
- Try connecting another network device to the fiber optic port using a different cable. If the port can establish a link, then the problem is with the cable or remote network device.
- Use the switch's management software to verify that the port is enabled.
- If the remote network device is a managed device, use its management firmware to determine whether its port is enabled.
- If the problem is with two BiDi (bi-directional) transceivers, refer to their data sheets to confirm that their transmission and reception frequencies are opposite each other. For example, a BiDi transceiver that transmits and receives at 1310nm and 1550nm, respectively, has to be connected to a transceiver that transmits and receives at 1550nm and 1310nm, respectively. Two BiDi transceivers that transmit and receive at the same frequencies will not establish a link.
- Test the attenuation on both directions on the fiber optic cable with a fiber optic tester to determine whether the optical signal is too weak (sensitivity) or too strong (maximum input power).

Problem 4: The switch functions intermittently.

Solutions: Check the system hardware status through the AlliedWare Plus management software:

- Use the SHOW SYSTEM ENVIRONMENT command in the Privileged Exec mode to verify that the input voltage from the power source to the switch is stable and within the approved operating range. The unit will shut down if the input voltage fluctuates above or below the approved operating range.
- Verify that the location of the switch allows for adequate airflow. The unit will shut down if it overheats.

Problem 5: The Switch ID LED on the front of the switch is flashing the letter "F."

Solutions: The switch is overheating and may have to shut down. The switch's location is not providing sufficient airflow for ventilation and cooling.

Chapter 11: Troubleshooting

This appendix contains the following sections:

- □ "Physical Specifications" on page 130
- □ "Environmental Specifications" on page 134
- □ "Power Specifications" on page 135
- □ "Certifications" on page 137
- □ "RJ-45 Copper Port Pinouts" on page 139
- □ "RJ-45 Style Serial Console Port Pinouts" on page 140

Physical Specifications

Dimensions

Table 7, Figure 80, and Figure 81 on page 131 list the dimensions of the switches.

Table 7. Product Dimensions (H x W x D)

x330-10GTX	3.8 cm x 26.3 cm x 17.9 cm (1.5 in. x 10.4 in. x 7.0 in.)
x330-20GTX and x330-28GTX	4.4 cm x 34.1 cm x 23.1 cm (1.7 in. x 13.4 in. x 9.1 in.)
x330-52GTX	4.4 cm x 44.1 cm x 32.2 cm (1.7 in. x 17.3 in. x 12.7 in.)

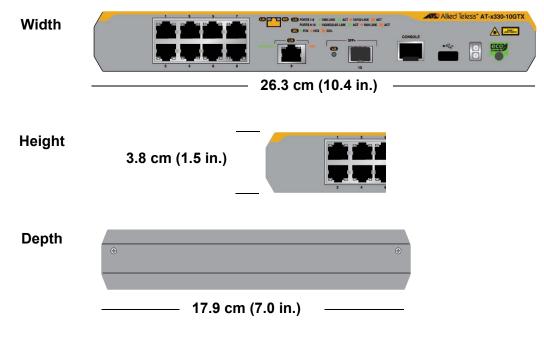


Figure 80. Dimensions of the x330-10GTX Switch

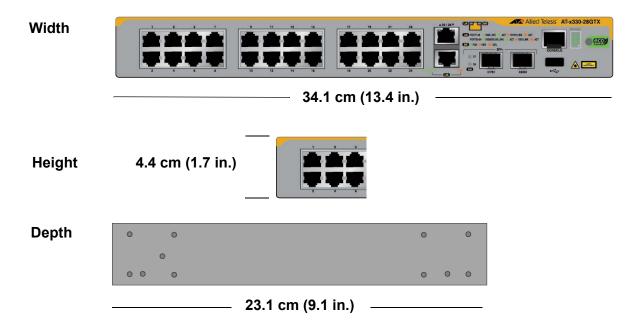


Figure 81. Dimensions of x330-20GTX and x330-28GTX Switches

Width

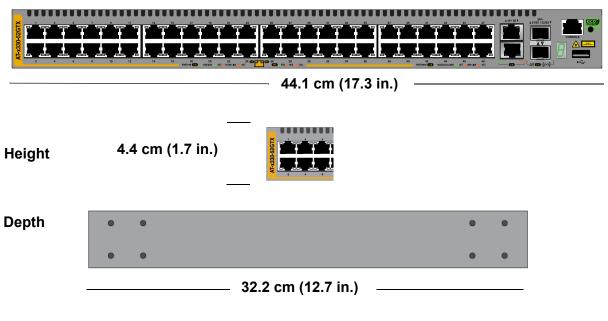


Figure 82. Dimensions of the x330-52GTX Switch

Weights

Table 8 lists the switch weights.

Table 8. Switch Weights

x330-10GTX	1.6 kg (3.53 lb.)
x330-20GTX	3.0 kg (6.61 lb.)
x330-28GTX	3.1 kg (6.84 lb.)
x330-52GTX	4.5 kg (9.92 lb.)

Ventilation

Table 9 lists the ventilation requirements.

Table 9. Ventilation Requirements

Recommended Minimum Ventilation on All Sides	10 cm (4.0 in)
---	----------------

Screw Hole Locations

Measurements in Figure 83 are in millimeters (mm).

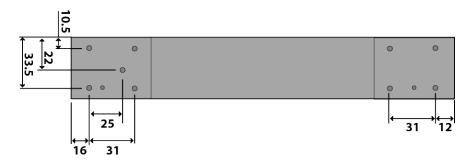


Figure 83. Bracket Screw Holes on the x330-20GTX and x330-28GTX Switches

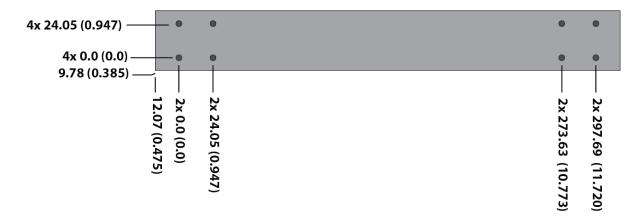


Figure 84. Bracket Screw Holes on the x330-52GTX Switch

Environmental Specifications

Table 10 lists the environmental specifications of the switches.

Table 10. Environmental Specifications

x330-10GTX, x330-20GTX, and x330-28GTX Switches Operating Temperature Range without SFP+ Transceivers	0° C to 50° C (32° F to 122° F)
x330-10GTX, x330-20GTX, and x330-28GTX Switches Operating Temperature Range with SFP+ Transceivers	0° C to 45° C (32° F to 113° F)
x330-52GTX Switch Operating Temperature Range with and without SFP+ Transceivers	0° C to 50° C (32° F to 122° F)
x330-52GTX Switch Noise Level ¹	 <42 dB when outside temperature is less than 30° C (86° F) >42 dB when outside temperature is greater than 30° C (86° F)
Storage Temperature	-25° C to 70° C (-13° F to 158° F)
Operating Humidity	5% to 90% noncondensing
Storage Humidity	5% to 95% noncondensing
Maximum Operating Altitude	3,000 m (9,842 ft)
Maximum Nonoperating Altitude	4,000 m (13,100 ft)

1. The x330-52GTX Switch has a single fan inside the back panel. The x330-10GTX, x330-20GTX, and x330-28GTX Switches are fanless.

Power Specifications

This section contains the maximum power consumption values, input voltages, and heat dissipation values.

Maximum Power Consumptions

Table 11 lists the maximum power consumptions of the switch.

 Table 11. Maximum Power Consumption

x330-10GTX	21 watts
x330-20GTX	28 watts
x330-28GTX	33 watts
x330-52GTX	52 watts

Input Voltages

Table 12 lists the input voltage of the switch.

Table 12. Input Voltages

x330-10GTX	100-240 VAC~, 0.5A maximum, 50/60 Hz
x330-20GTX	100-240 VAC~, 0.7A maximum, 50/60 Hz
x330-28GTX	100-240 VAC~, 0.8A maximum, 50/60 Hz
x330-52GTX	100-240 VAC~, 0.7A maximum, 50/60 Hz

Note

The input voltage, current, and frequency can be found on the rating label on the bottom panel of the switch.

Heat Dissipation

Table 13 lists the heat dissipation.

Table 13. Heat Dissipation

x330-10GTX	71 BTU/hr
x330-20GTX	96 BTU/hr
x330-28GTX	114 BTU/hr
x330-52GTX	181 BTU/hr

Certifications

Table 14 lists the product certificates.

Table 14. Product Certifications

1	
CISPR Class A (Comité International Spécial des Perturbations Radioélectriques)	
Compliant with European and China RoHS standards	
RCM (Regulatory Compliance Mark)	
NIAP (National Information Assurance Partnership)	
CE (Conformité Européenne)	
WEEE (Waste Electrical and Electronic Equipment)	
RoHS (EU 1025/863) (Restriction of Hazardous Substances)	
EMC (Immunity): EN 55024, EN 55035	
Laser Safety: EN 60825-1	
EN 55032 Class A, EN 61000-3-2, EN 61000-3-3	
Electrical Safety: EN 62368-1 (UL/ EN/IEC)	
TEC (Telecommunications Engineering Center)	
VCCI Class A (Voluntary Control Council for Interference)	

Mexico	NOM (Normas Oficiales Mexicanas)	
North America	FCC Class A	
	Laser Safety: EN 60825-1	
	_C UL _{US}	
	Energy Star	
United Kingdom	UKCA (UK Conformity Assessment)	

Table 14. Product Certifications (Con	tinued)
Table 14. Froduct Certifications (Con	unued)

RJ-45 Copper Port Pinouts

Figure 85 illustrates the pin layout of the RJ-copper ports.




Figure 85. Pin Layout for the RJ-45 Copper Ports (Front View)

Table 15 lists the pin signals for the copper ports.

Table 15. Pin Signals for Copper Ports

Pin	10/100Mbps MDI	10/100Mbps MDI-X	1/2.5/5/10Gbps
1	TX+	RX+	Bi-directional pair A+
2	TX-	RX-	Bi-directional pair A-
3	RX+	TX+	Bi-directional pair B+
4	Not used	Not used	Bi-directional pair C+
5	Not used	Not used	Bi-directional pair C-
6	RX-	TX-	Bi-directional pair B-
7	Not used	Not used	Bi-directional pair D+
8	Not used	Not used	Bi-directional pair D-

RJ-45 Style Serial Console Port Pinouts

Table 16 lists the pin signals of the RJ-45 style serial Console port.

Pin	Signal
1	Unused
2	Unused
3	Transmit Data
4	Signal Ground
5	Signal Ground
6	Receive Data
7	Unused
8	Unused
9	N/A

Table 16. RJ-45 Style Serial Console Port Pin Signals